

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021422\
Data File : FF009942.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2022 18:09
Operator : AJ\MA
Sample : PB142653BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 15 00:44:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.417	2288887	21.177 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.468	51195	0.441 ug/ml
14) N-DOTRIACONTANE	18.298	70735	0.611 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021422\
Data File : FF009942.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2022 18:09
Operator : AJ\MA
Sample : PB142653BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 15 00:44:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

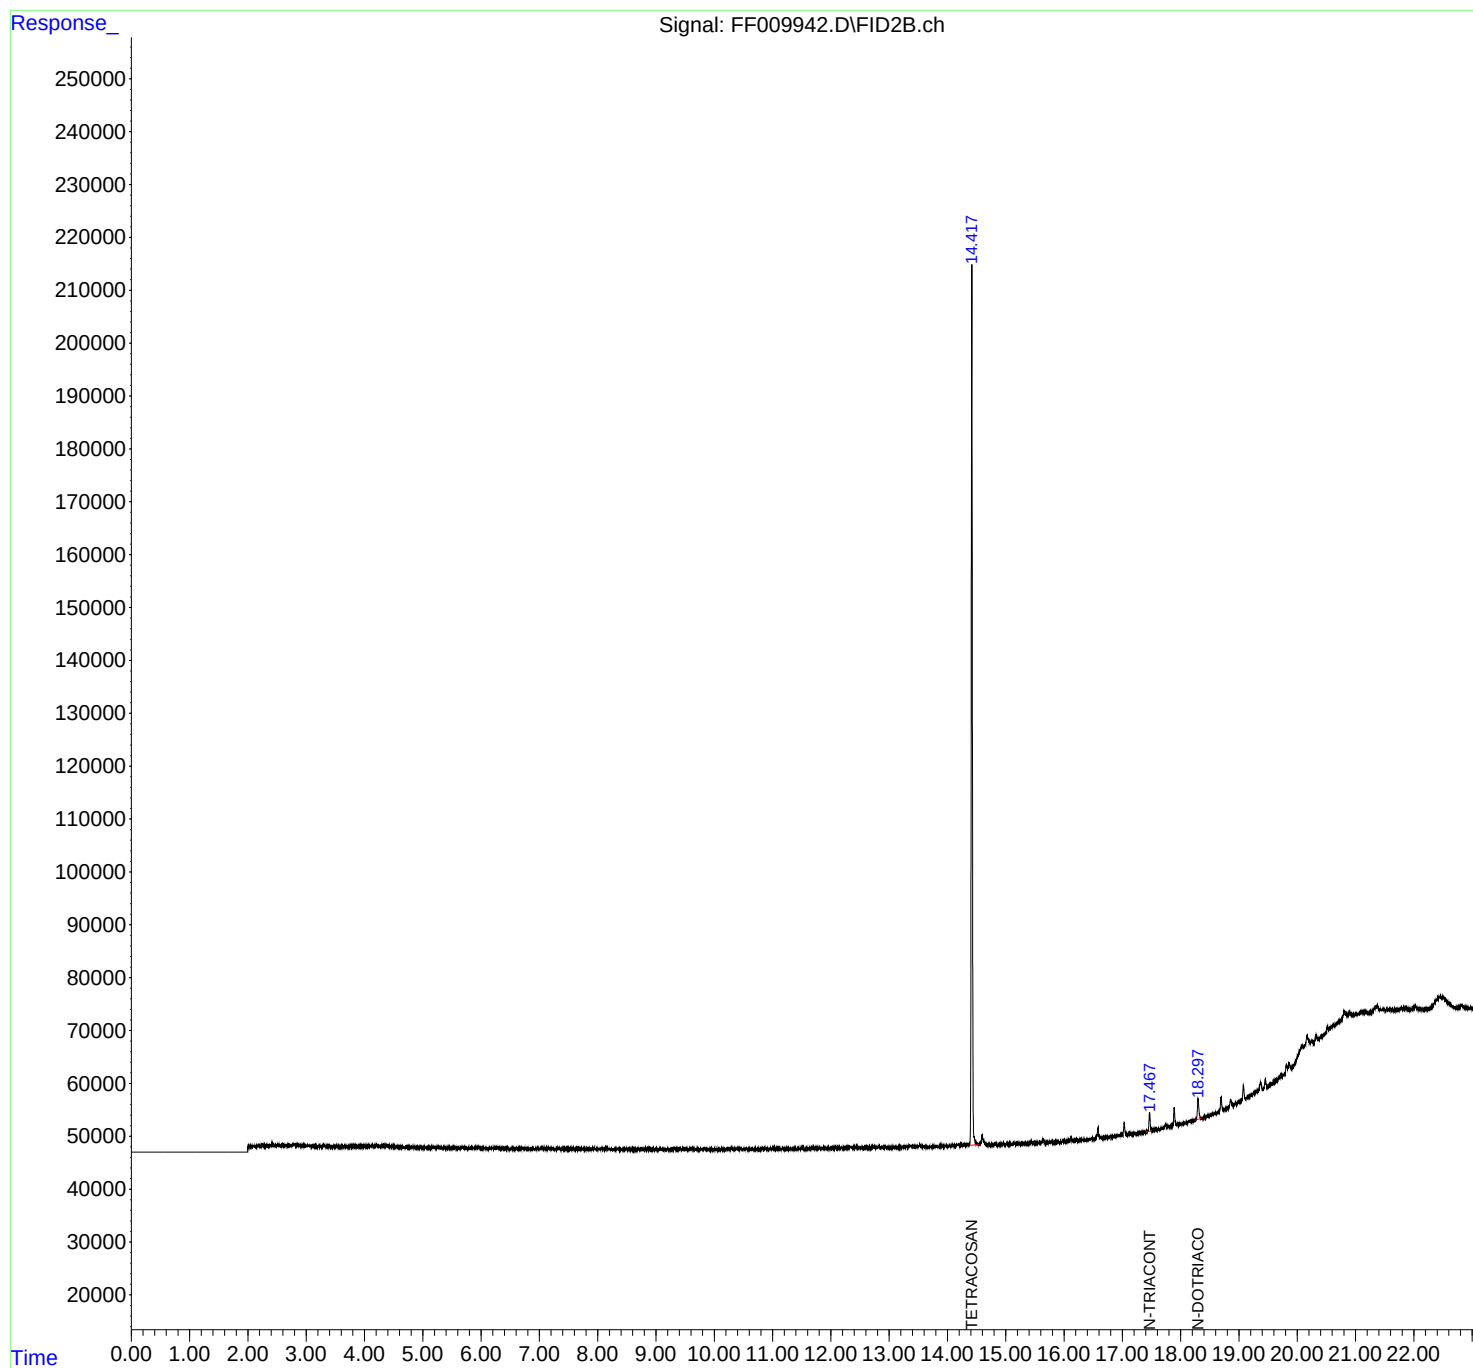


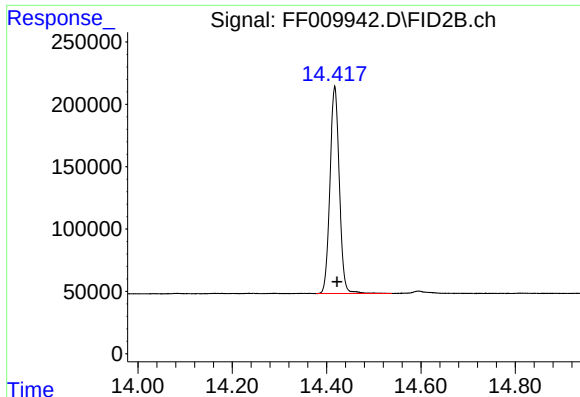

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.417 min
Delta R.T.: -0.005 min
Response: 2288887
Conc: 21.18 ug/ml

Instrument :
FID_F
ClientSampleId :

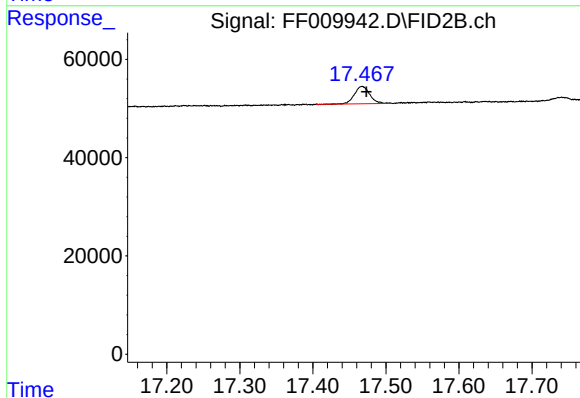

#13 N-TRIACONTANE

R.T.: 17.468 min
Delta R.T.: -0.006 min
Response: 51195
Conc: 0.44 ug/ml

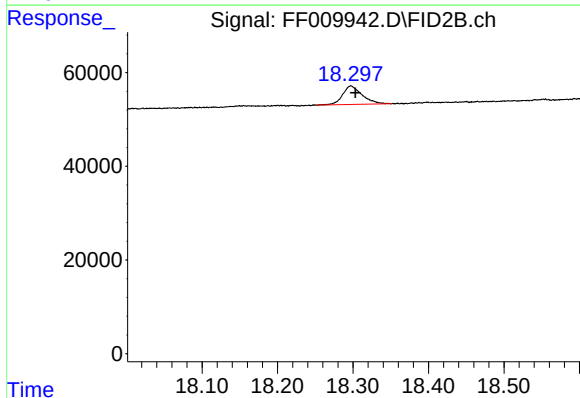

#14 N-DOTRIACONTANE

R.T.: 18.298 min
Delta R.T.: -0.006 min
Response: 70735
Conc: 0.61 ug/ml