

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021423\
 Data File : FF012070.D
 Signal(s) : FID2B.ch
 Acq On : 14 Feb 2023 12:26
 Operator : YP\AJ
 Sample : PB150831BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 14 16:44:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
 Quant Title :
 QLast Update : Fri Jan 27 14:21:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.050	1889335	16.396 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.945	60764	0.467 ug/ml
15) N-TETRATRIACONTANE	19.728	167352	1.503 ug/ml
16) N-HEXATRIACONTANE	20.470	112429	1.094 ug/ml
17) N-OCTATRIACONTANE	21.211	63500	0.645 ug/ml
18) N-TETRACONTANE	22.135	58312	0.563 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021423\
Data File : FF012070.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2023 12:26
Operator : YP\AJ
Sample : PB150831BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 14 16:44:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

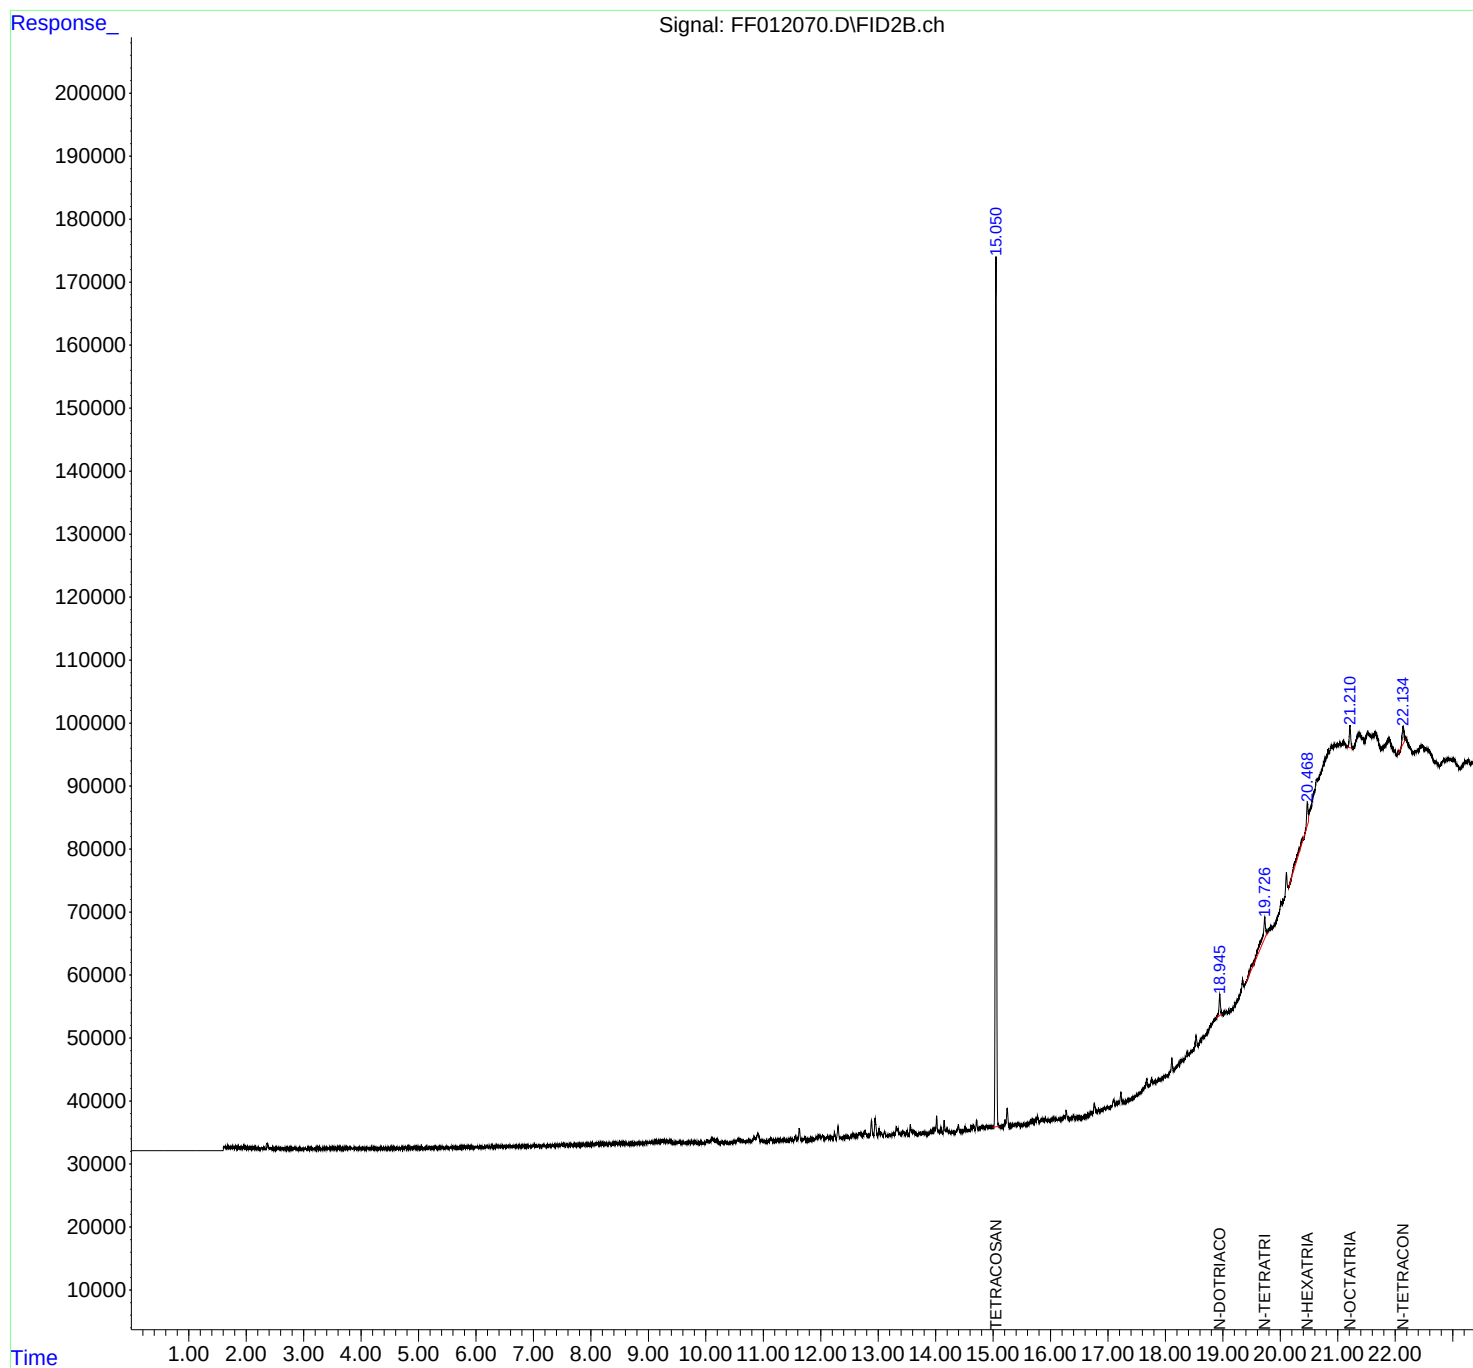


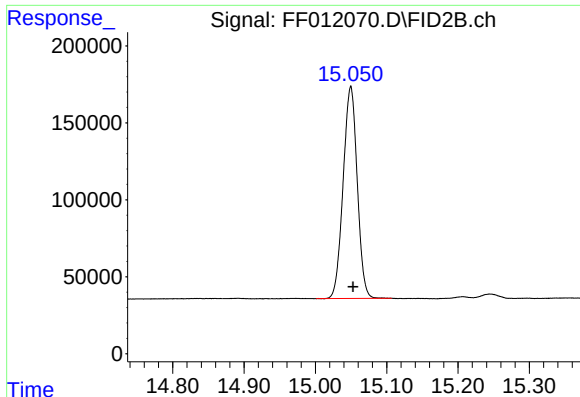

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.050 min
Delta R.T.: -0.003 min
Response: 1889335
Conc: 16.40 ug/ml

Instrument :
FID_F
ClientSampleId :

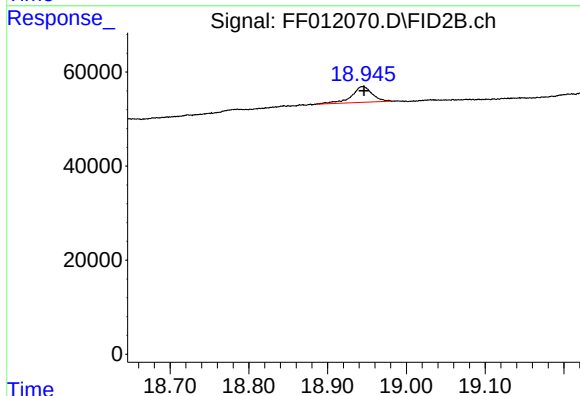


#14 N-DOTRIACONTANE

R.T.: 18.945 min
Delta R.T.: -0.001 min
Response: 60764
Conc: 0.47 ug/ml

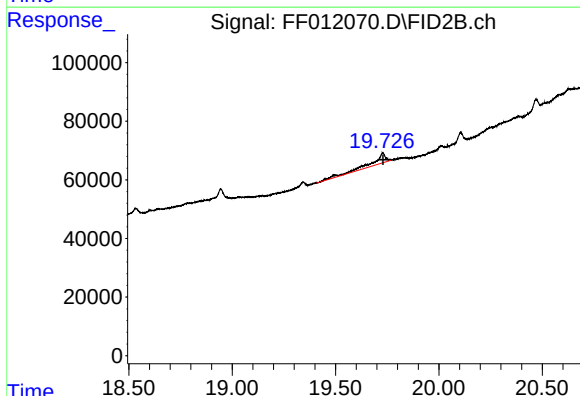


#15 N-TETRATRIACONTANE

R.T.: 19.728 min
Delta R.T.: -0.002 min
Response: 167352
Conc: 1.50 ug/ml

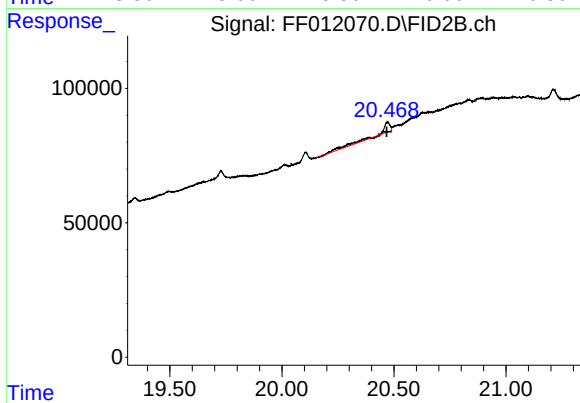

#16 N-HEXATRIACONTANE


R.T.: 20.470 min
Delta R.T.: 0.002 min
Response: 112429
Conc: 1.09 ug/ml

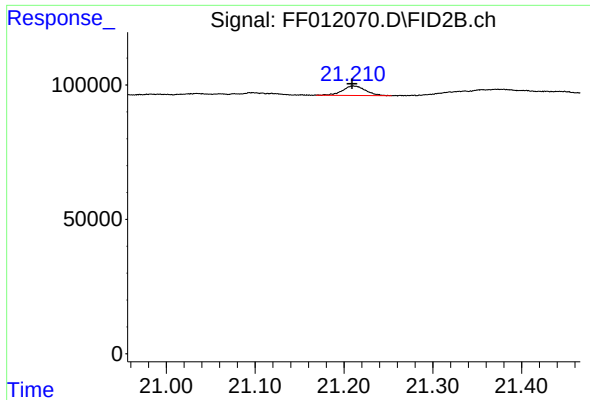

#17 N-OCTATRIACONTANE

R.T.: 21.211 min
Delta R.T.: 0.002 min
Response: 63500
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

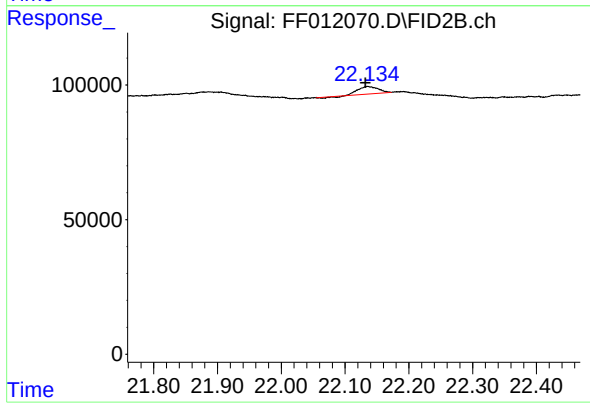

#18 N-TETRACONTANE

R.T.: 22.135 min
Delta R.T.: 0.003 min
Response: 58312
Conc: 0.56 ug/ml