

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF021423\  
 Data File : FF012075.D  
 Signal(s) : FID2B.ch  
 Acq On : 14 Feb 2023 14:54  
 Operator : YP\AJ  
 Sample : 01529-09  
 Misc :  
 ALS Vial : 60 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 SB-05-COMP

Manual Integrations  
 APPROVED

Reviewed By :Ankita  
 Jodhani

Integration File: Sample.e  
 Quant Time: Feb 14 16:45:26 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF012723.M  
 Quant Title :  
 QLast Update : Fri Jan 27 14:21:25 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

02/15/2023  
 Supervised By :Sohil  
 Jodhani

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----02/15/2023               |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 15.055 | 2680508  | 23.262 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF021423\  
Data File : FF012075.D  
Signal(s) : FID2B.ch  
Acq On : 14 Feb 2023 14:54  
Operator : YP\AJ  
Sample : 01529-09  
Misc :  
ALS Vial : 60 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
SB-05-COMP


Manual Integrations  
APPROVED


Reviewed By :Ankita  
Jodhani

Integration File: Sample.e  
Quant Time: Feb 14 16:45:26 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF012723.M  
Quant Title :  
QLast Update : Fri Jan 27 14:21:25 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

02/15/2023  
Supervised By :Sohil  
Jodhani

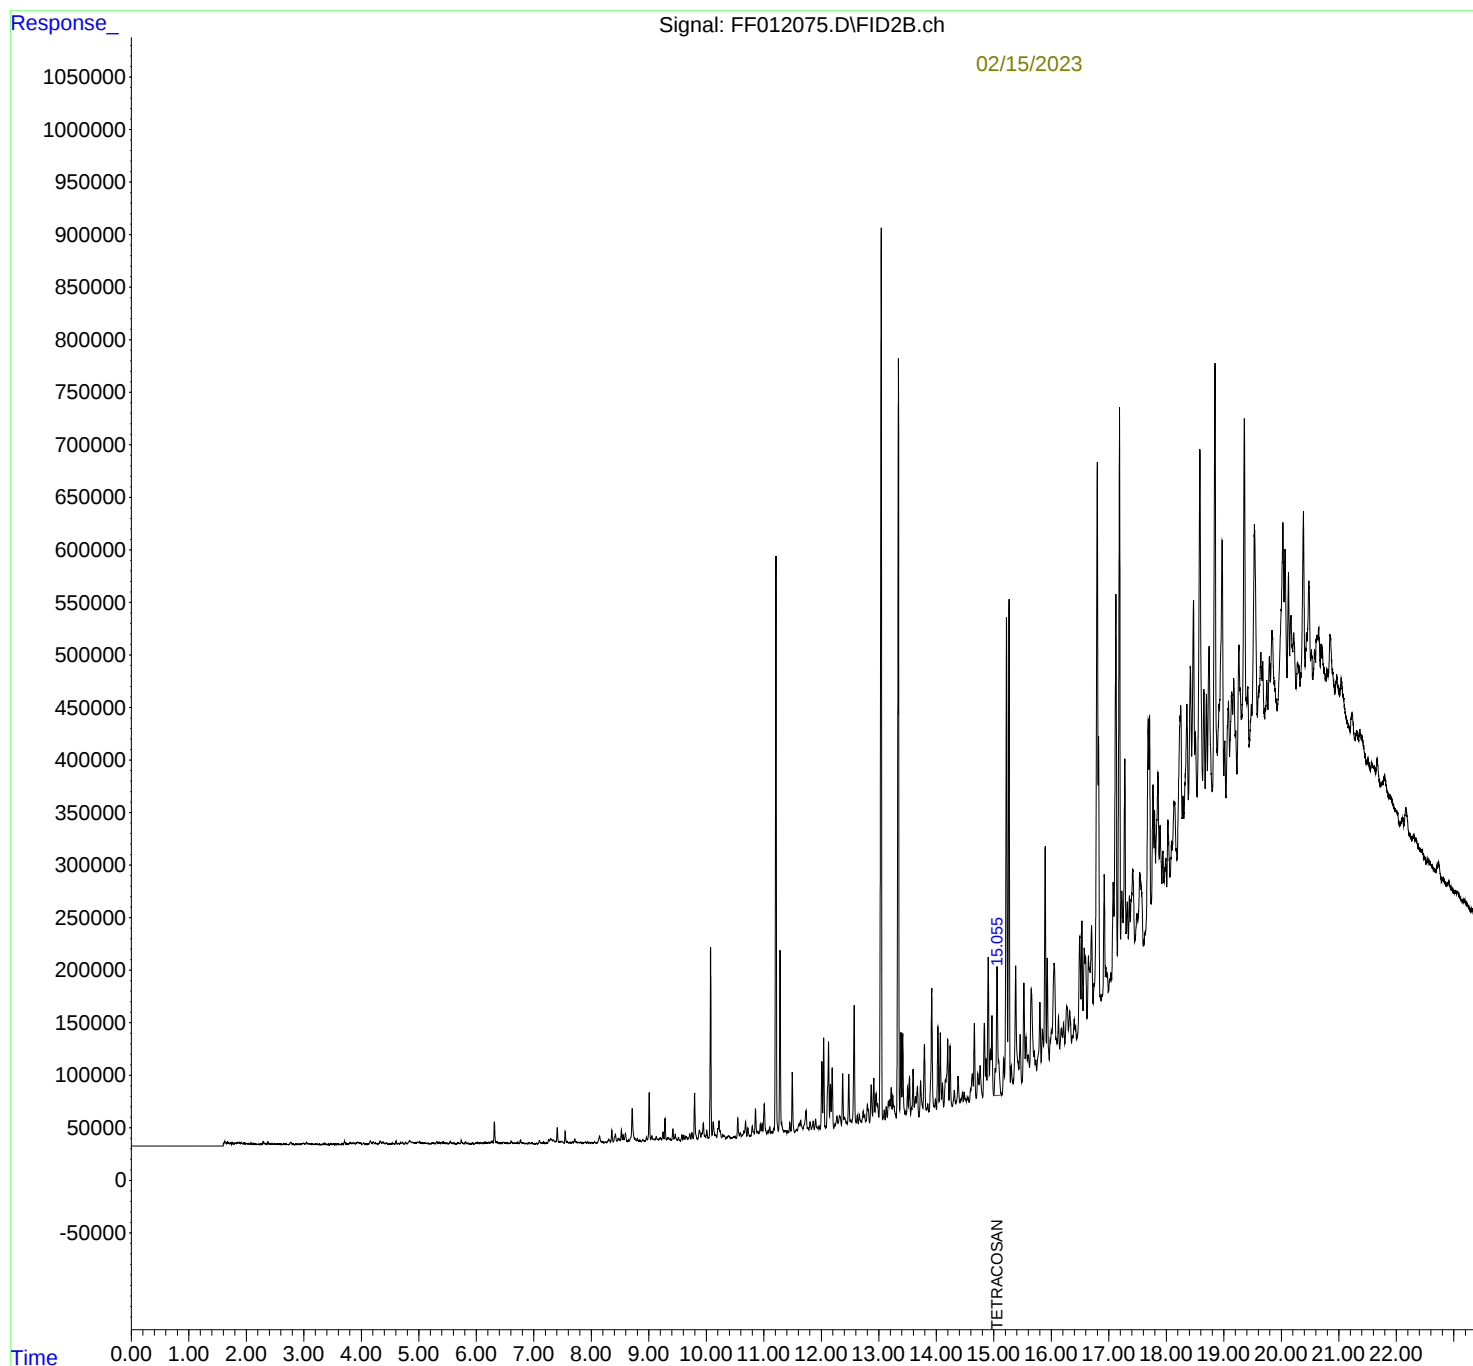

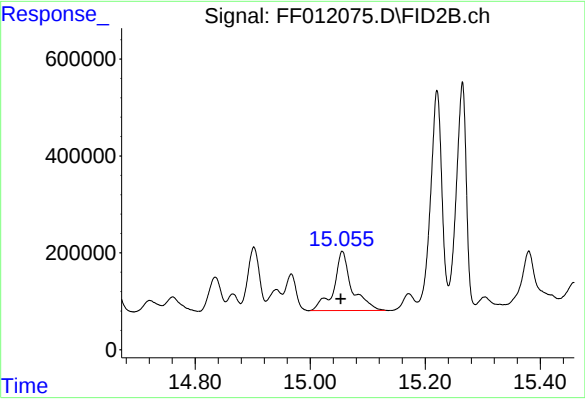

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.055 min  
Delta R.T.: 0.002 min  
Response: 2680508  
Conc: 23.26 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
SB-05-COMP

Manual Integrations  
APPROVED

Reviewed By :Ankita  
Jodhani

02/15/2023  
Supervised By :Sohil  
Jodhani

02/15/2023