

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021519\
 Data File : FF003527.D
 Signal(s) : FID2B.ch
 Acq On : 15 Feb 2019 16:42
 Operator : AJ\SJ
 Sample : K1346-15 2X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 15 22:37:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.614	800776	6.633 ug/ml
Target Compounds			
7) N-EICOSANE	12.509	94829	0.690 ug/ml
8) N-DOCOSANE	13.711	133471	0.976 ug/ml
10) N-TETRACOSANE	14.817	130846	0.962 ug/ml
11) N-HEXACOSANE	15.844	281103	2.072 ug/ml
12) N-OCTACOSANE	16.798	565649	4.131 ug/ml
13) N-TRIACONTANE	17.689	710537	5.032 ug/ml
14) N-DOTRIACONTANE	18.526	526281	3.814 ug/ml
15) N-TETRATRIACONTANE	19.316	319520	2.519 ug/ml
16) N-HEXATRIACONTANE	20.059	218031	1.865 ug/ml
17) N-OCTATRIACONTANE	20.806	489525	4.529 ug/ml
18) N-TETRACONTANE	21.703	110973	1.025 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021519\
Data File : FF003527.D
Signal(s) : FID2B.ch
Acq On : 15 Feb 2019 16:42
Operator : AJ\SJ
Sample : K1346-15 2X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 15 22:37:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

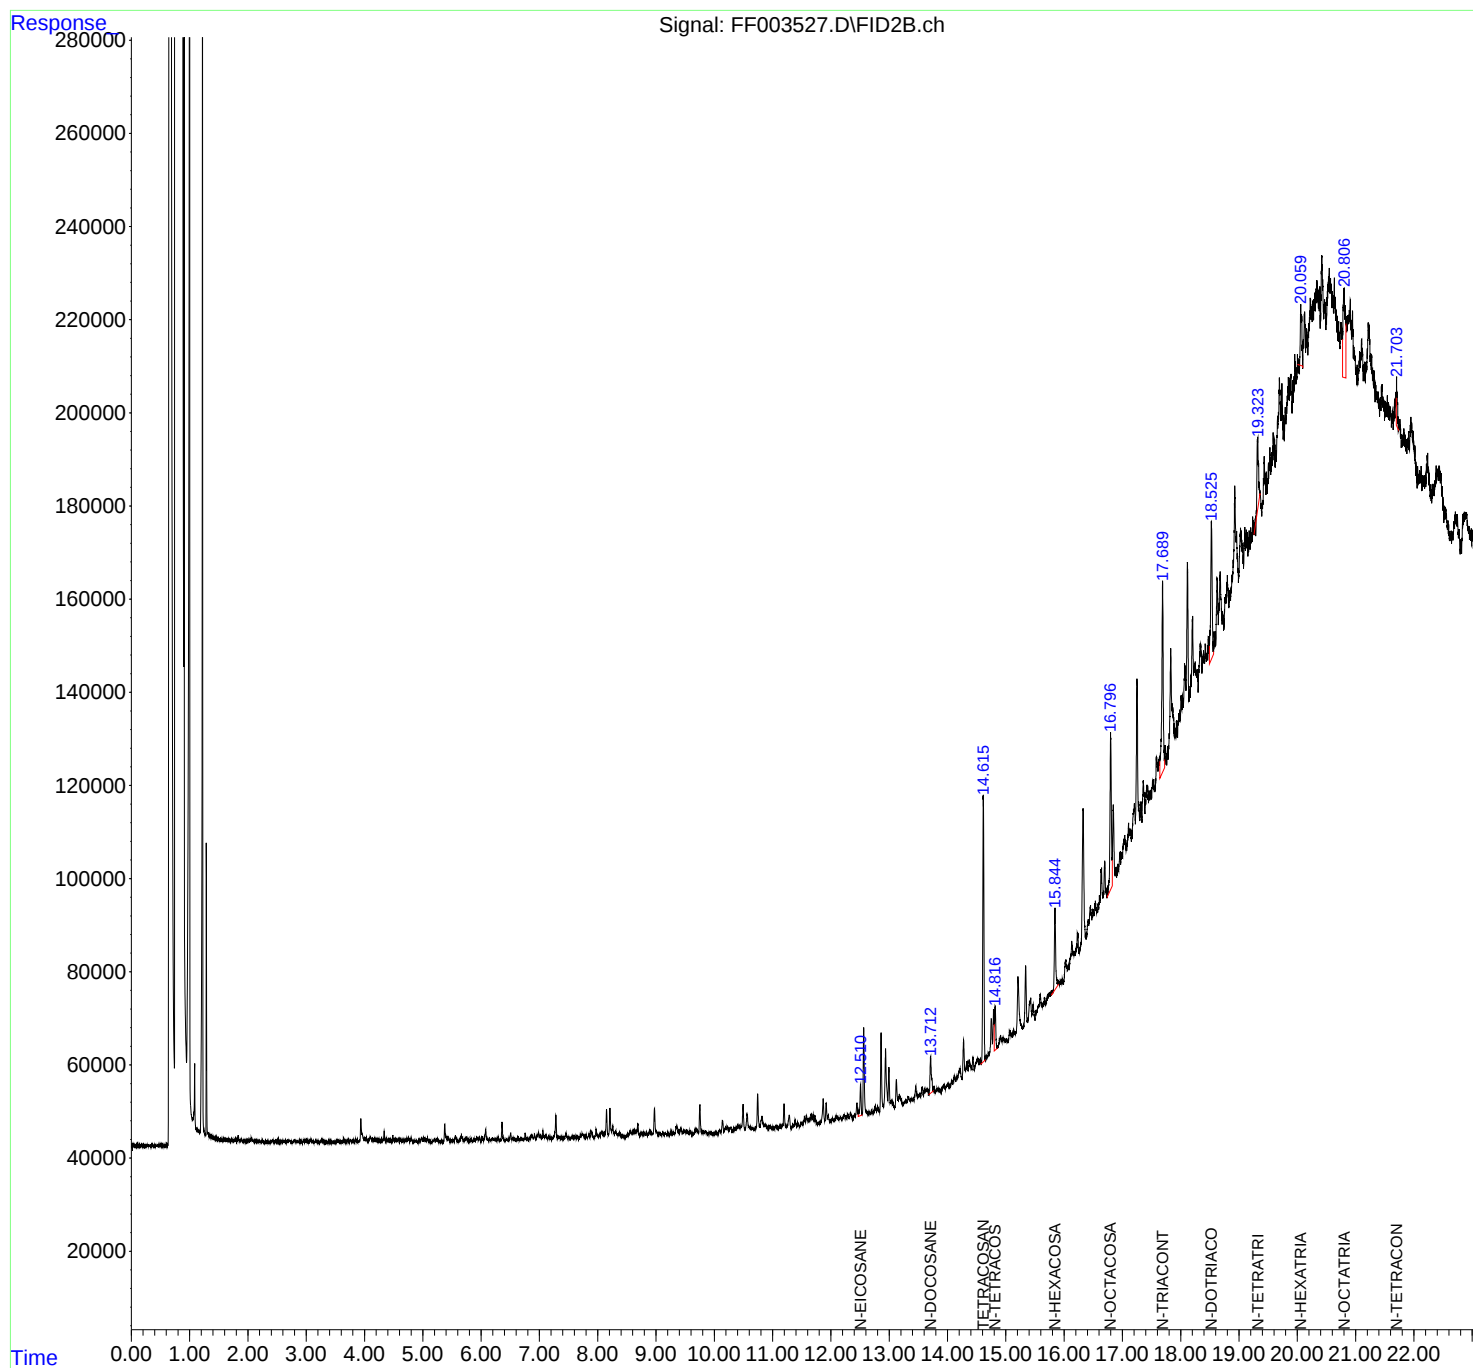

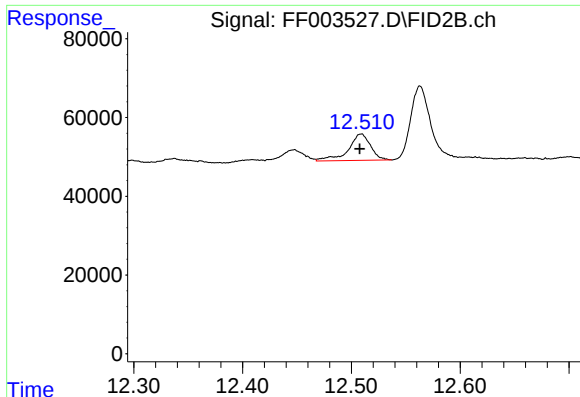


#7 N-EICOSANE

R.T.: 12.509 min
Delta R.T.: 0.001 min
Response: 94829
Conc: 0.69 ug/ml

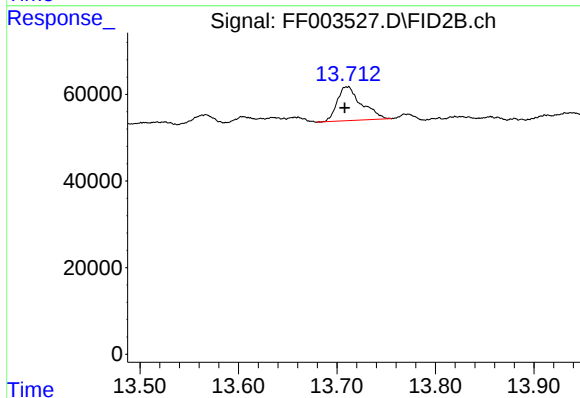


#8 N-DOCOSANE

R.T.: 13.711 min
Delta R.T.: 0.003 min
Response: 133471
Conc: 0.98 ug/ml

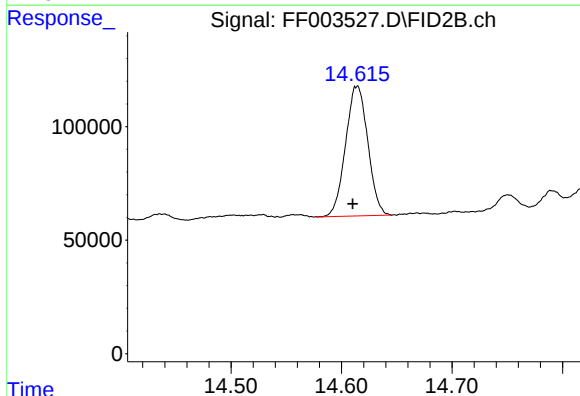


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.614 min
Delta R.T.: 0.004 min
Response: 800776
Conc: 6.63 ug/ml

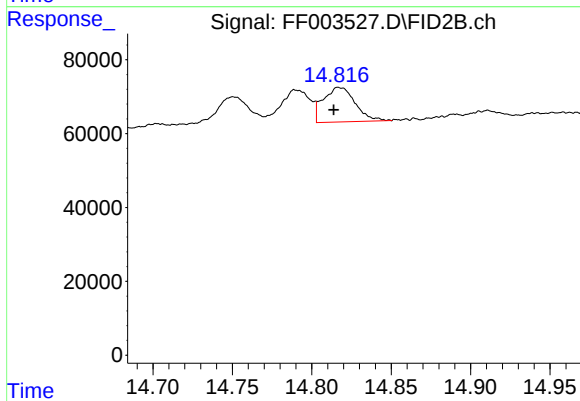


#10 N-TETRACOSANE

R.T.: 14.817 min
Delta R.T.: 0.004 min
Response: 130846
Conc: 0.96 ug/ml

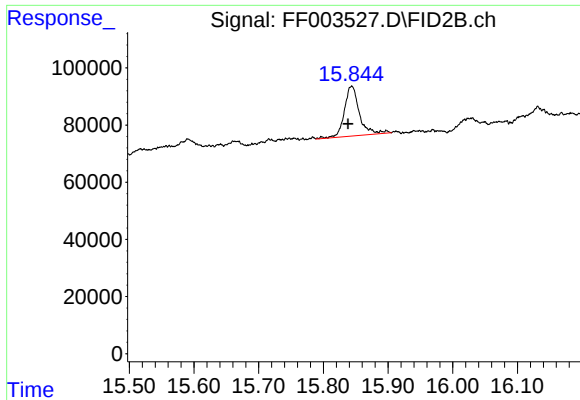


#11 N-HEXACOSANE

R.T.: 15.844 min
Delta R.T.: 0.005 min
Response: 281103
Conc: 2.07 ug/ml

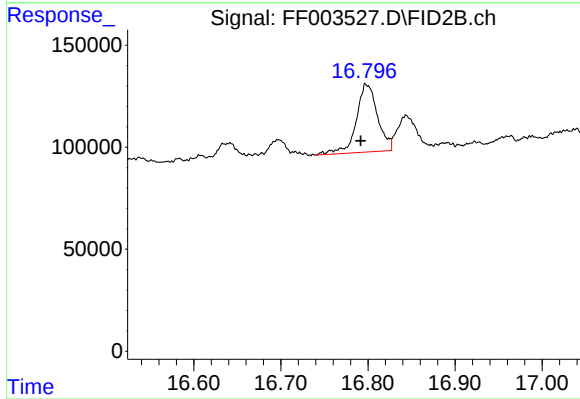


#12 N-OCTACOSANE

R.T.: 16.798 min
Delta R.T.: 0.006 min
Response: 565649
Conc: 4.13 ug/ml

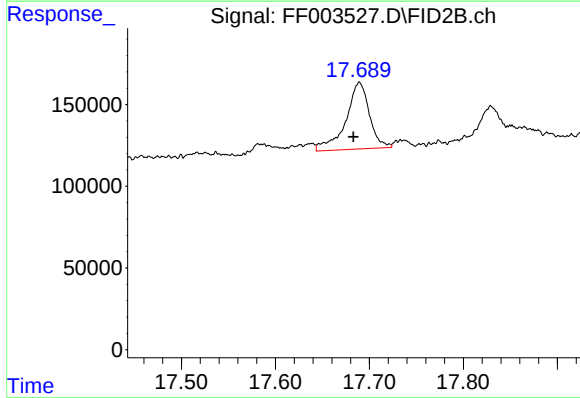


#13 N-TRIACONTANE

R.T.: 17.689 min
Delta R.T.: 0.006 min
Response: 710537
Conc: 5.03 ug/ml

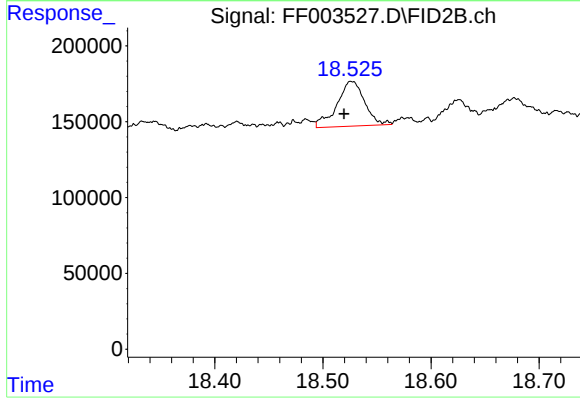

#14 N-DOTRIACONTANE

R.T.: 18.526 min
Delta R.T.: 0.007 min
Response: 526281
Conc: 3.81 ug/ml

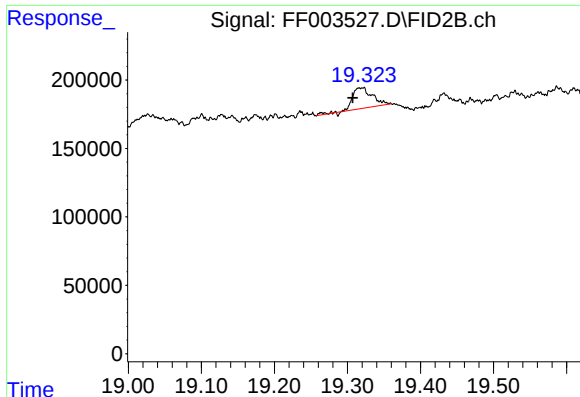


#15 N-TETRATRIACONTANE

R.T.: 19.316 min

Delta R.T.: 0.009 min

Response: 319520

Conc: 2.52 ug/ml

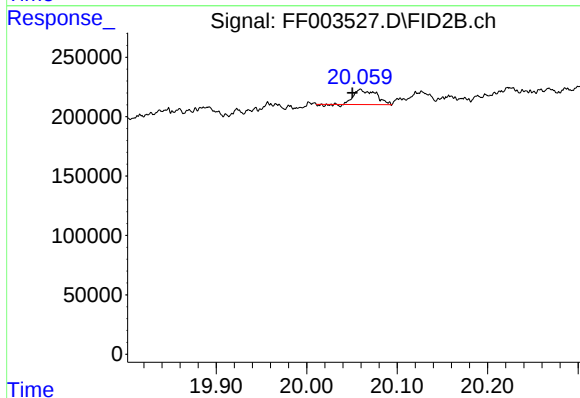


#16 N-HEXATRIACONTANE

R.T.: 20.059 min

Delta R.T.: 0.009 min

Response: 218031

Conc: 1.87 ug/ml

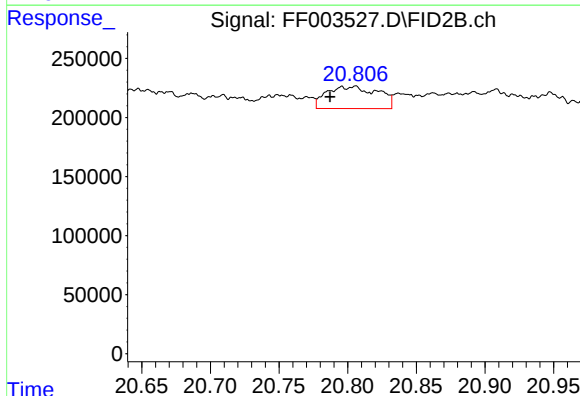


#17 N-OCTATRIACONTANE

R.T.: 20.806 min

Delta R.T.: 0.018 min

Response: 489525

Conc: 4.53 ug/ml

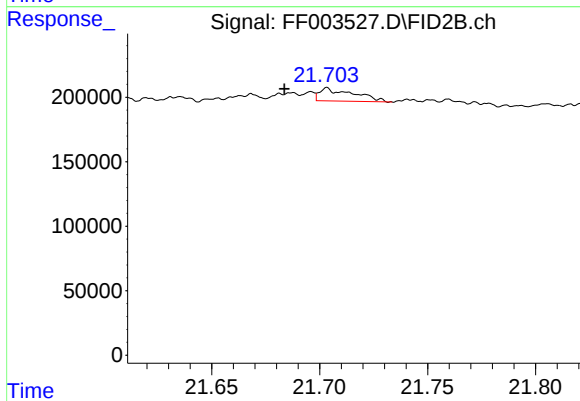

#18 N-TETRACONTANE

R.T.: 21.703 min

Delta R.T.: 0.020 min

Response: 110973

Conc: 1.02 ug/ml