

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021519\
Data File : FF003533.D
Signal(s) : FID2B.ch
Acq On : 15 Feb 2019 20:13
Operator : AJ\SJ
Sample : K1484-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 15 22:38:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.610	2073420	17.174 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.209f	230911	1.706 ug/ml
10)	N-TETRACOSANE	14.812	132849	0.977 ug/ml
11)	N-HEXACOSANE	15.838	210009	1.548 ug/ml
12)	N-OCTACOSANE	16.791	410242	2.996 ug/ml
13)	N-TRIACONTANE	17.682	475201	3.366 ug/ml
14)	N-DOTRIACONTANE	18.518	275482	1.996 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021519\
Data File : FF003533.D
Signal(s) : FID2B.ch
Acq On : 15 Feb 2019 20:13
Operator : AJ\SJ
Sample : K1484-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 15 22:38:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

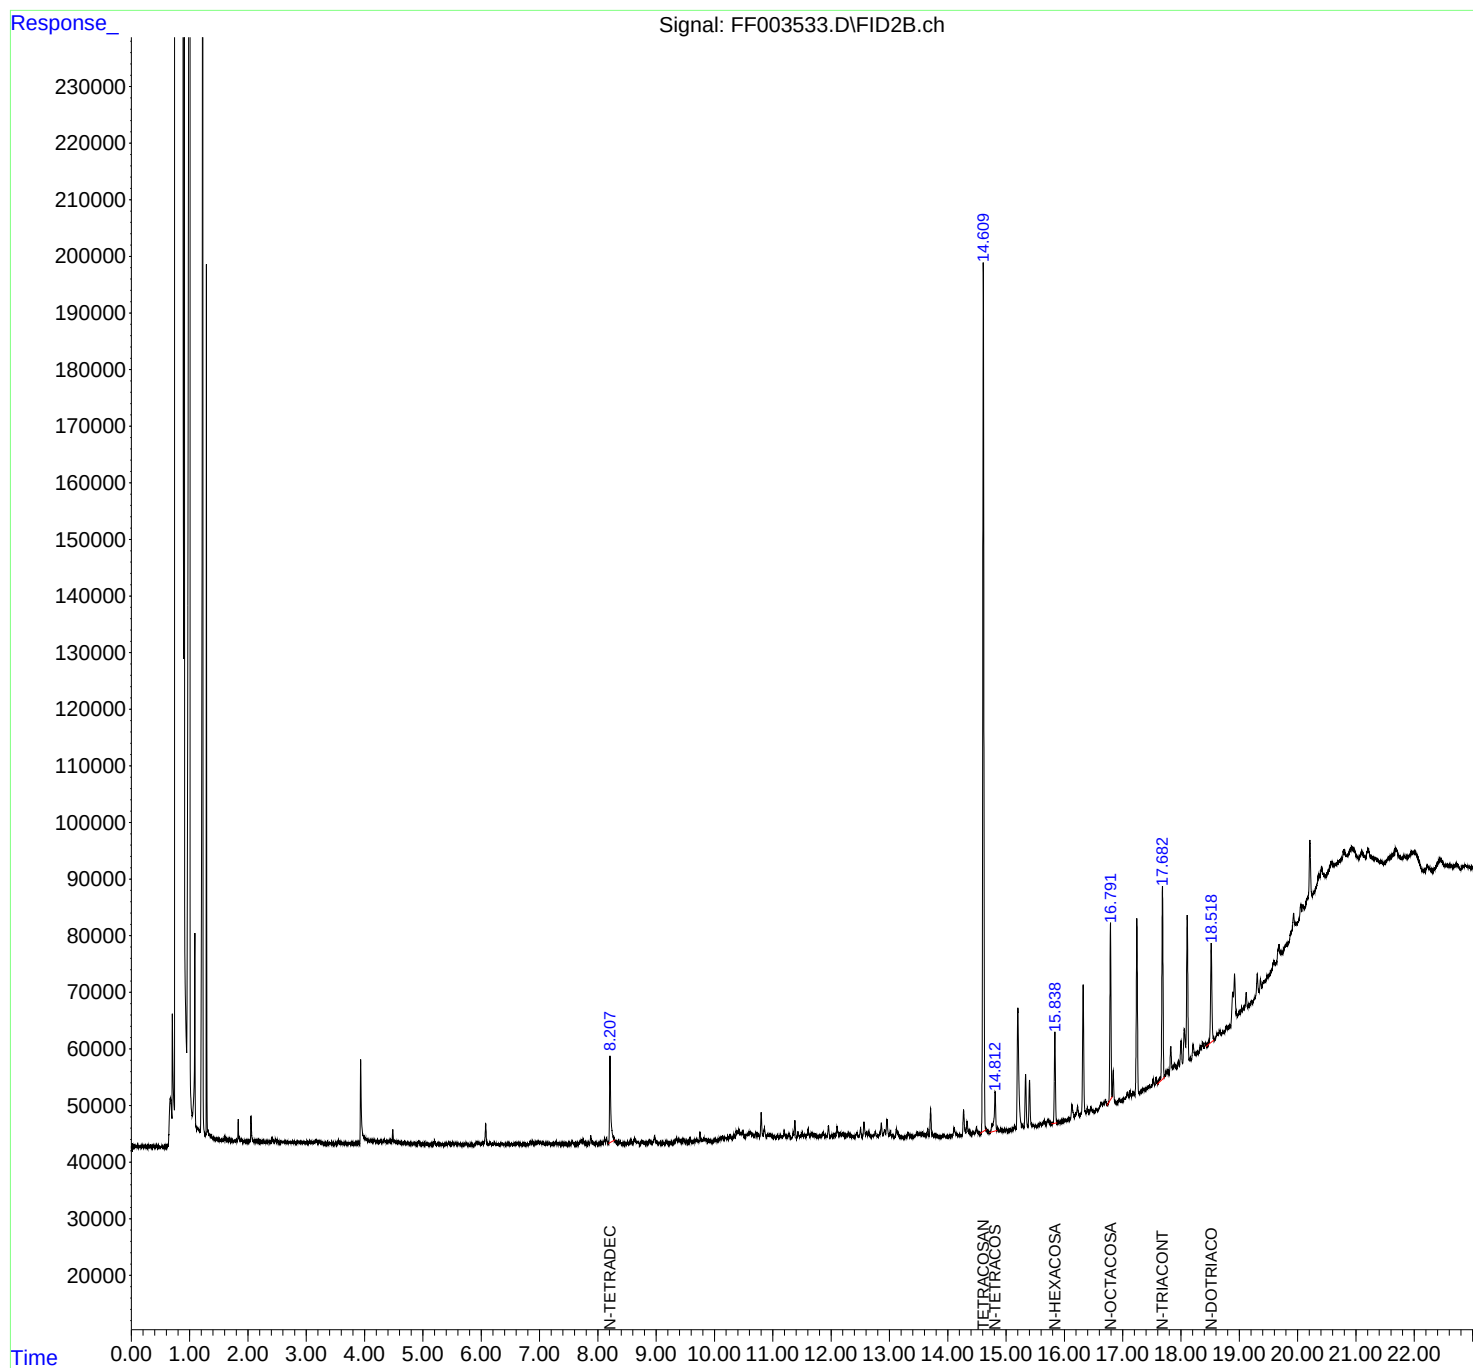

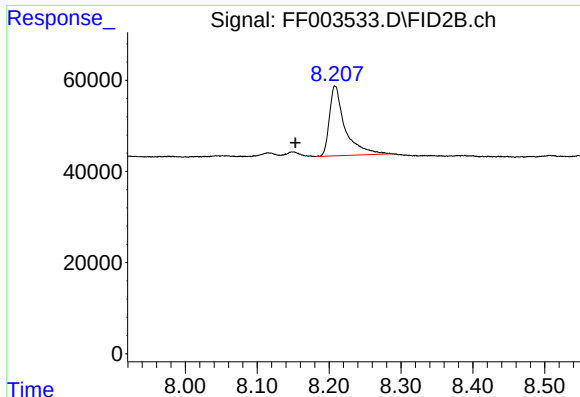


#4 N-TETRADECANE

R.T.: 8.209 min
Delta R.T.: 0.055 min
Response: 230911
Conc: 1.71 ug/ml

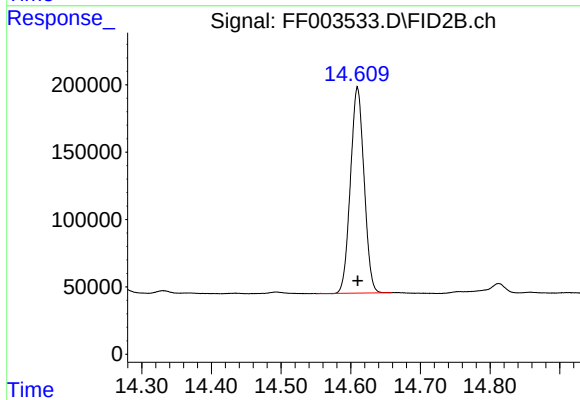


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.610 min
Delta R.T.: 0.000 min
Response: 2073420
Conc: 17.17 ug/ml

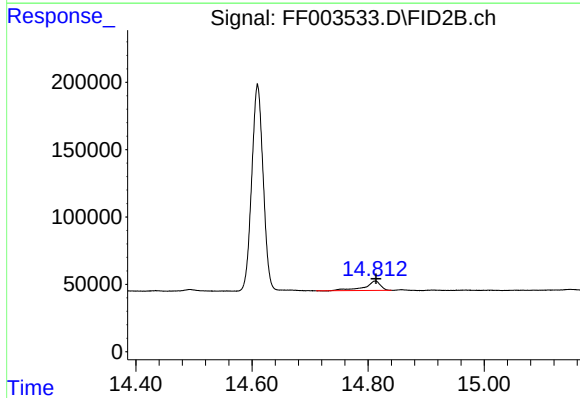


#10 N-TETRACOSANE

R.T.: 14.812 min
Delta R.T.: -0.001 min
Response: 132849
Conc: 0.98 ug/ml

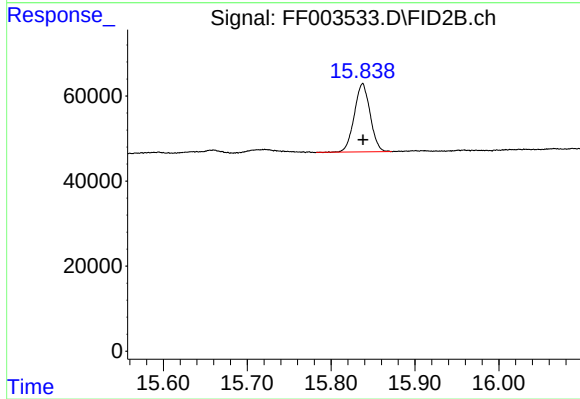


#11 N-HEXACOSANE

R.T.: 15.838 min
Delta R.T.: 0.000 min
Response: 210009
Conc: 1.55 ug/ml

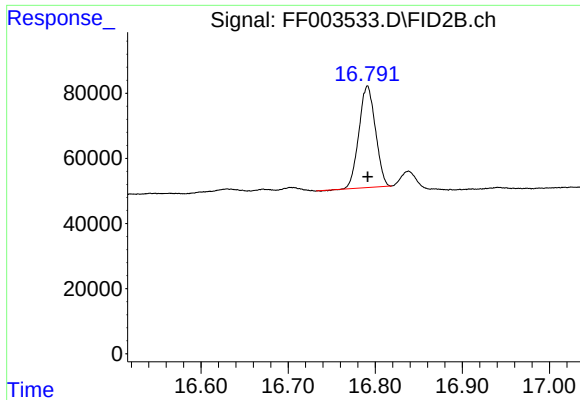


#12 N-OCTACOSANE

R.T.: 16.791 min
Delta R.T.: 0.000 min
Response: 410242
Conc: 3.00 ug/ml

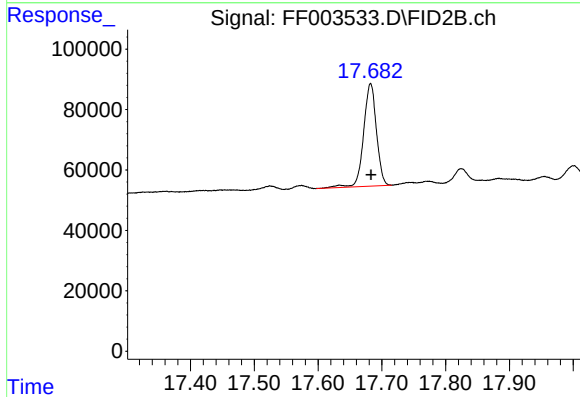

#13 N-TRIACONTANE

R.T.: 17.682 min
Delta R.T.: 0.000 min
Response: 475201
Conc: 3.37 ug/ml

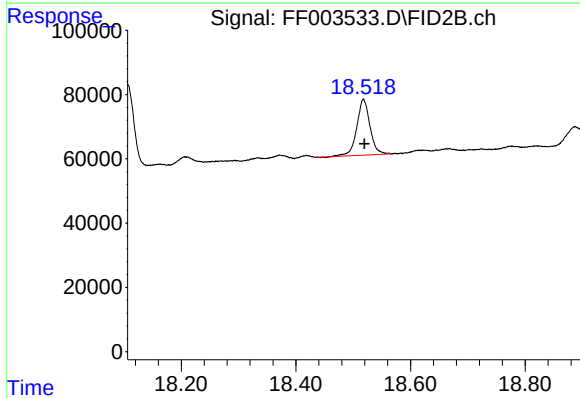

#14 N-DOTRIACONTANE

R.T.: 18.518 min
Delta R.T.: -0.002 min
Response: 275482
Conc: 2.00 ug/ml