

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF021623\  
 Data File : FF012118.D  
 Signal(s) : FID2B.ch  
 Acq On : 16 Feb 2023 09:26  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Feb 17 02:32:49 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF012723.M  
 Quant Title :  
 QLast Update : Fri Jan 27 14:21:25 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.062 | 1736816  | 15.072 ug/ml |
| Target Compounds              |        |          |              |
| 14) N-DOTRIACONTANE           | 18.950 | 80010    | 0.615 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.721 | 261552   | 2.349 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.469 | 799903   | 7.787 ug/ml  |
| 17) N-OCTATRIACONTANE         | 21.222 | 879343   | 8.927 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF021623\  
Data File : FF012118.D  
Signal(s) : FID2B.ch  
Acq On : 16 Feb 2023 09:26  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Feb 17 02:32:49 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF012723.M  
Quant Title :  
QLast Update : Fri Jan 27 14:21:25 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

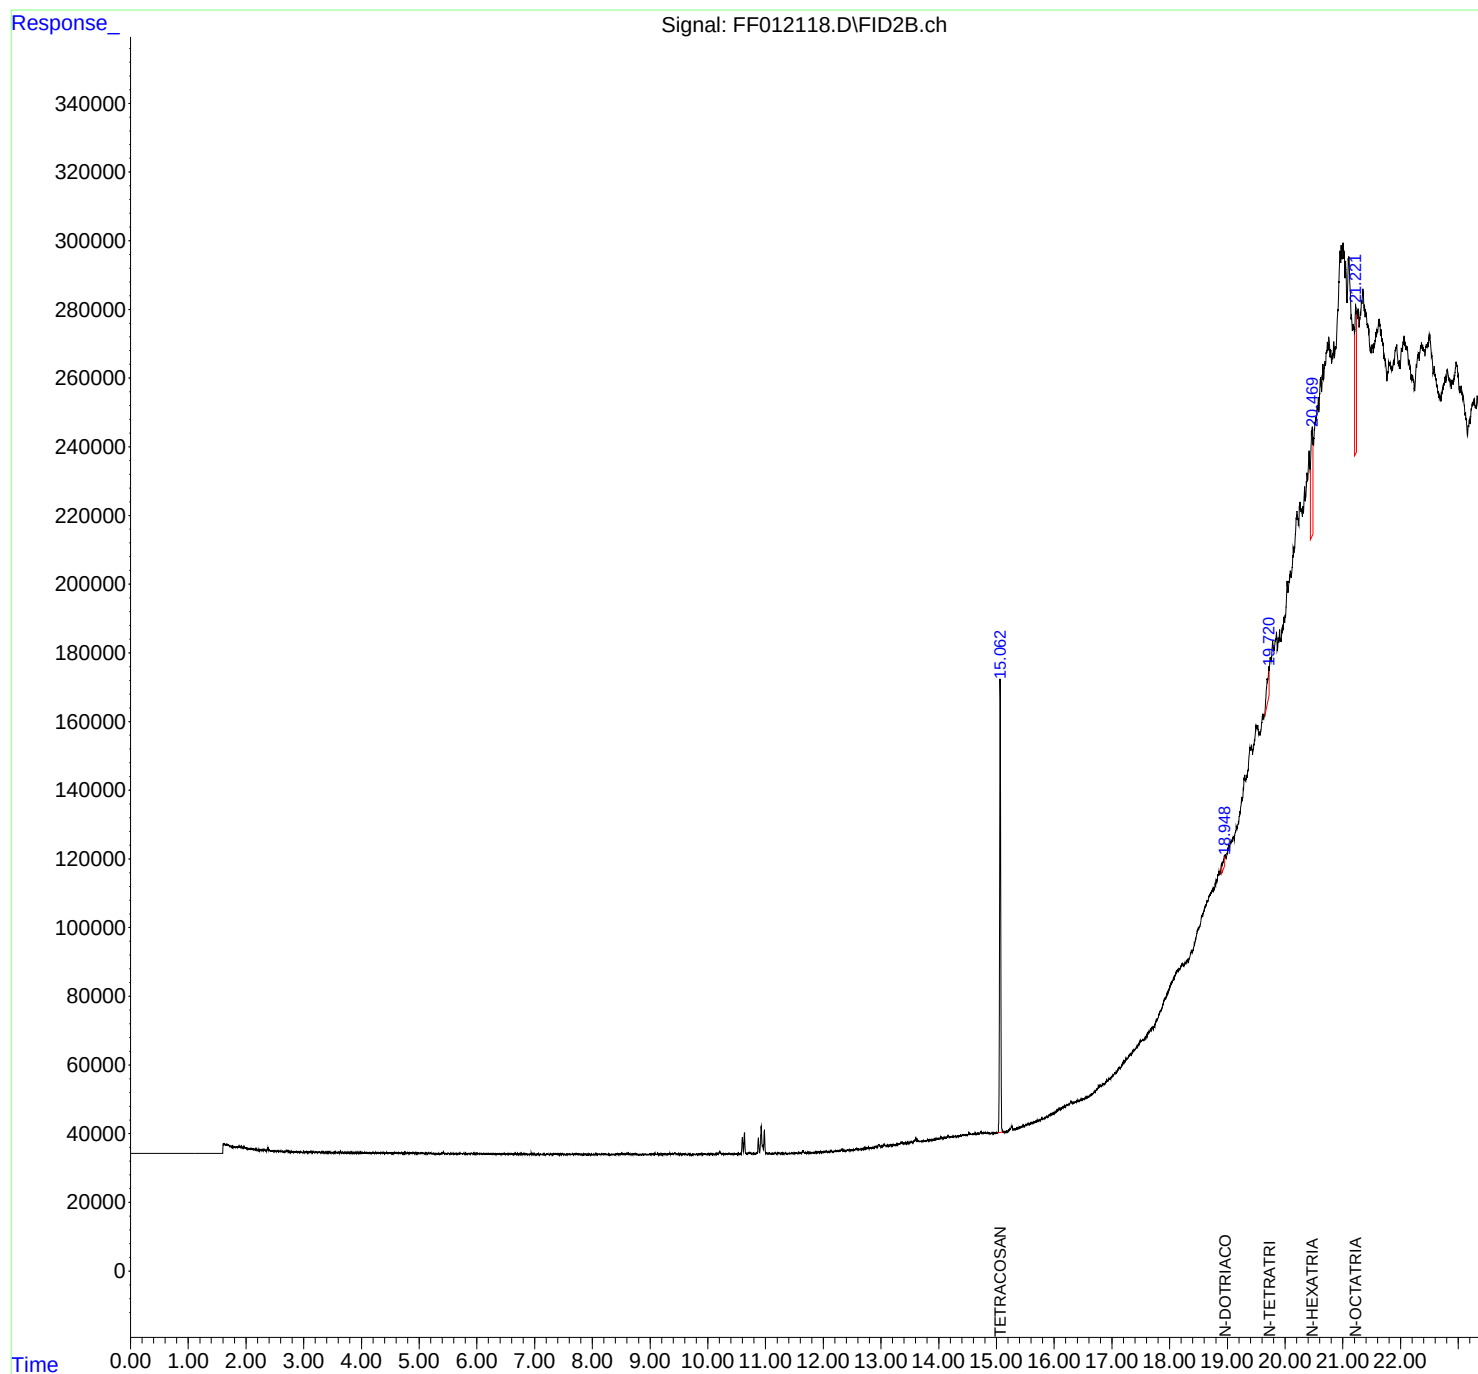


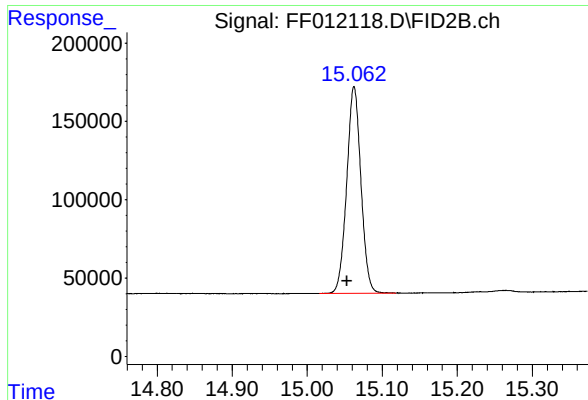

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.062 min  
Delta R.T.: 0.009 min  
Response: 1736816  
Conc: 15.07 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

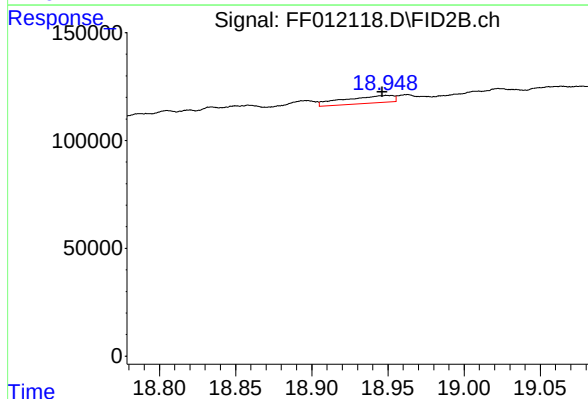


#14 N-DOTRIACONTANE

R.T.: 18.950 min  
Delta R.T.: 0.004 min  
Response: 80010  
Conc: 0.61 ug/ml

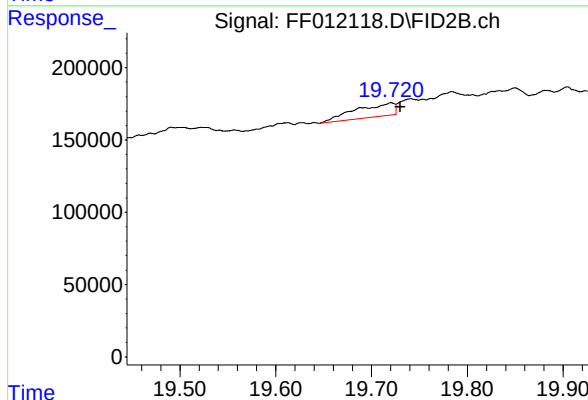


#15 N-TETRATRIACONTANE

R.T.: 19.721 min  
Delta R.T.: -0.009 min  
Response: 261552  
Conc: 2.35 ug/ml

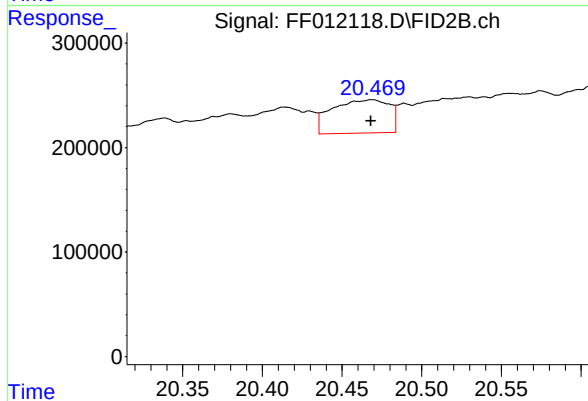

#16 N-HEXATRIACONTANE

R.T.: 20.469 min  
Delta R.T.: 0.000 min  
Response: 799903  
Conc: 7.79 ug/ml

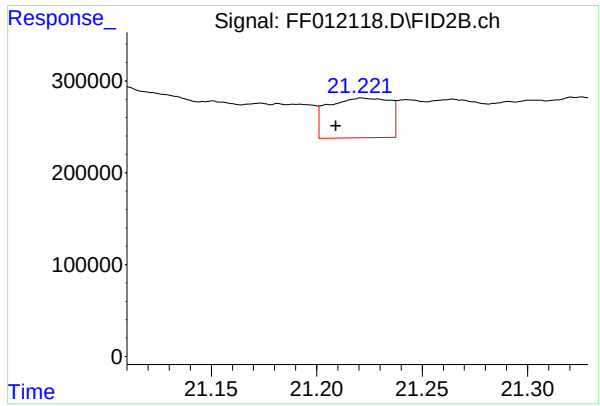

#17 N-OCTATRIACONTANE

R.T.: 21.222 min  
Delta R.T.: 0.012 min  
Response: 879343  
Conc: 8.93 ug/ml

Instrument :

FID\_F

ClientSampleId :