

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021623\
Data File : FF012120.D
Signal(s) : FID2B.ch
Acq On : 16 Feb 2023 10:25
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Feb 17 02:33:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.772	1623931	13.556 ug/ml
12) N-OCTACOSANE	17.237	1711058	13.158 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021623\
Data File : FF012120.D
Signal(s) : FID2B.ch
Acq On : 16 Feb 2023 10:25
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Feb 17 02:33:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

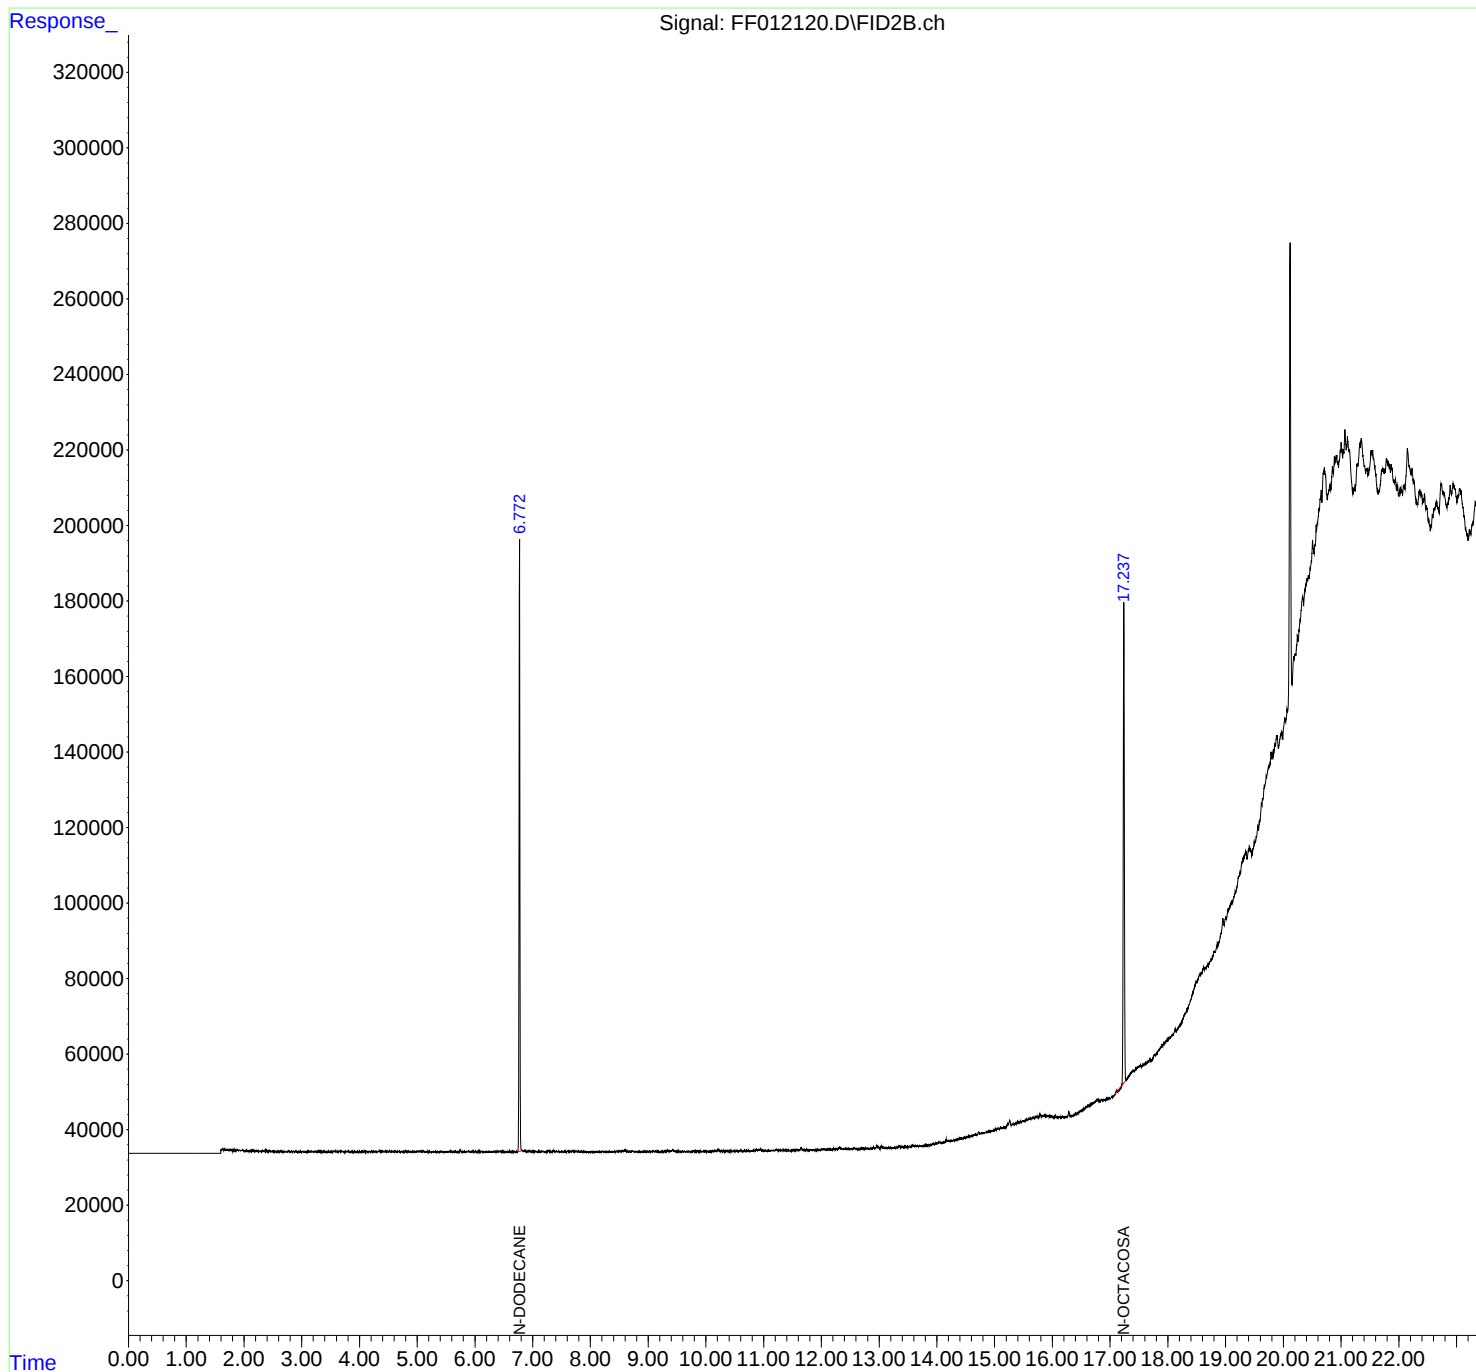


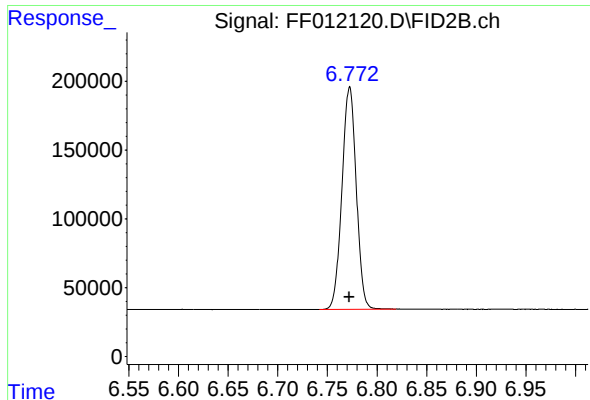

#3 N-DODECANE


R.T.: 6.772 min
Delta R.T.: 0.000 min
Response: 1623931
Conc: 13.56 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

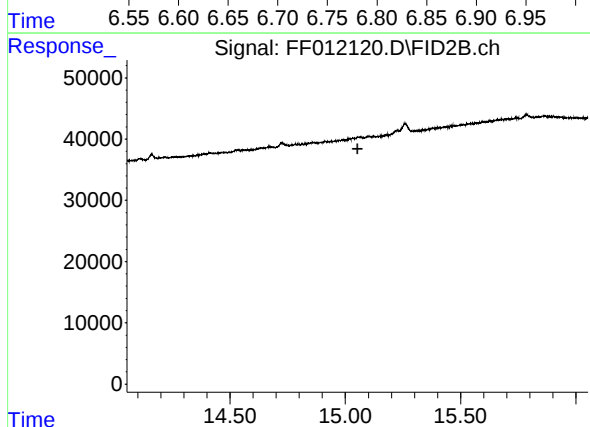

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.053 min
Response: 0
Conc: N.D.

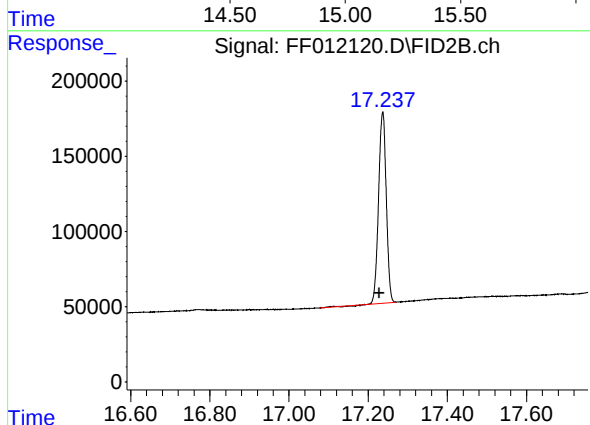

#12 N-OCTACOSANE

R.T.: 17.237 min
Delta R.T.: 0.009 min
Response: 1711058
Conc: 13.16 ug/ml