

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021623\
Data File : FF012135.D
Signal(s) : FID2B.ch
Acq On : 16 Feb 2023 18:34
Operator : YP\AJ
Sample : 01576-01
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RE137-BAGFILTER-20220215

Integration File: autoint1.e
Quant Time: Feb 17 02:34:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.064	1695682	14.715 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021623\
Data File : FF012135.D
Signal(s) : FID2B.ch
Acq On : 16 Feb 2023 18:34
Operator : YP\AJ
Sample : 01576-01
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RE137-BAGFILTER-20220215

Integration File: autoint1.e
Quant Time: Feb 17 02:34:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF012723.M
Quant Title :
QLast Update : Fri Jan 27 14:21:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

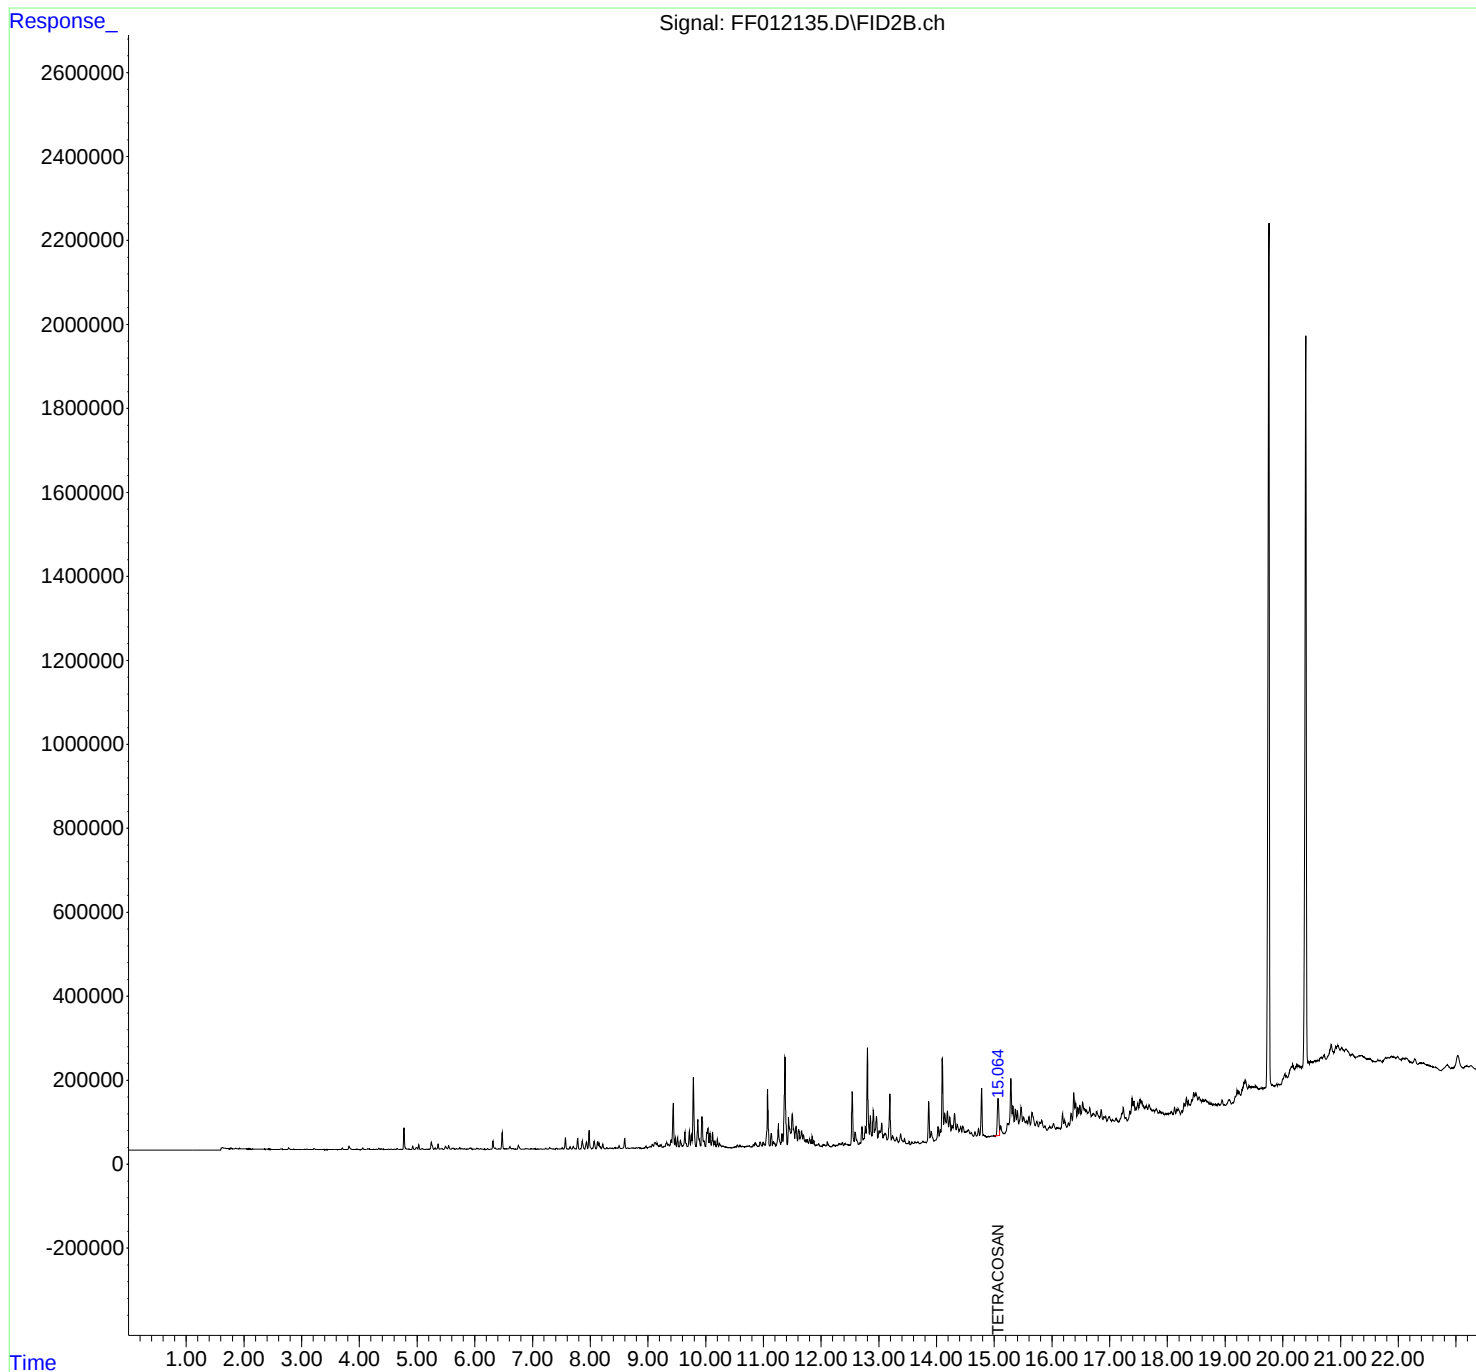

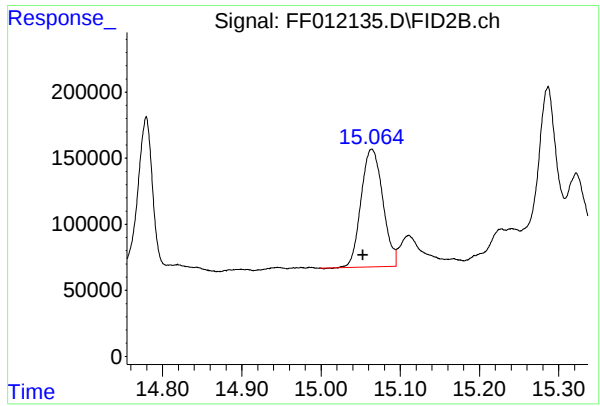

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.064 min
Delta R.T.: 0.011 min
Response: 1695682
Conc: 14.72 ug/ml

Instrument :
FID_F
ClientSampleId :
RE137-BAGFILTER-20220215