

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
Data File : FF006414.D
Signal(s) : FID2B.ch
Acq On : 17 Feb 2020 08:56
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 18 00:26:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.794	105679	0.756 ug/ml
14)	N-DOTRIACONTANE	18.490	64222	0.488 ug/ml
15)	N-TETRATRIACONTANE	19.269	351344	3.129 ug/ml
16)	N-HEXATRIACONTANE	20.034	151532	1.566 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
Data File : FF006414.D
Signal(s) : FID2B.ch
Acq On : 17 Feb 2020 08:56
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 18 00:26:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

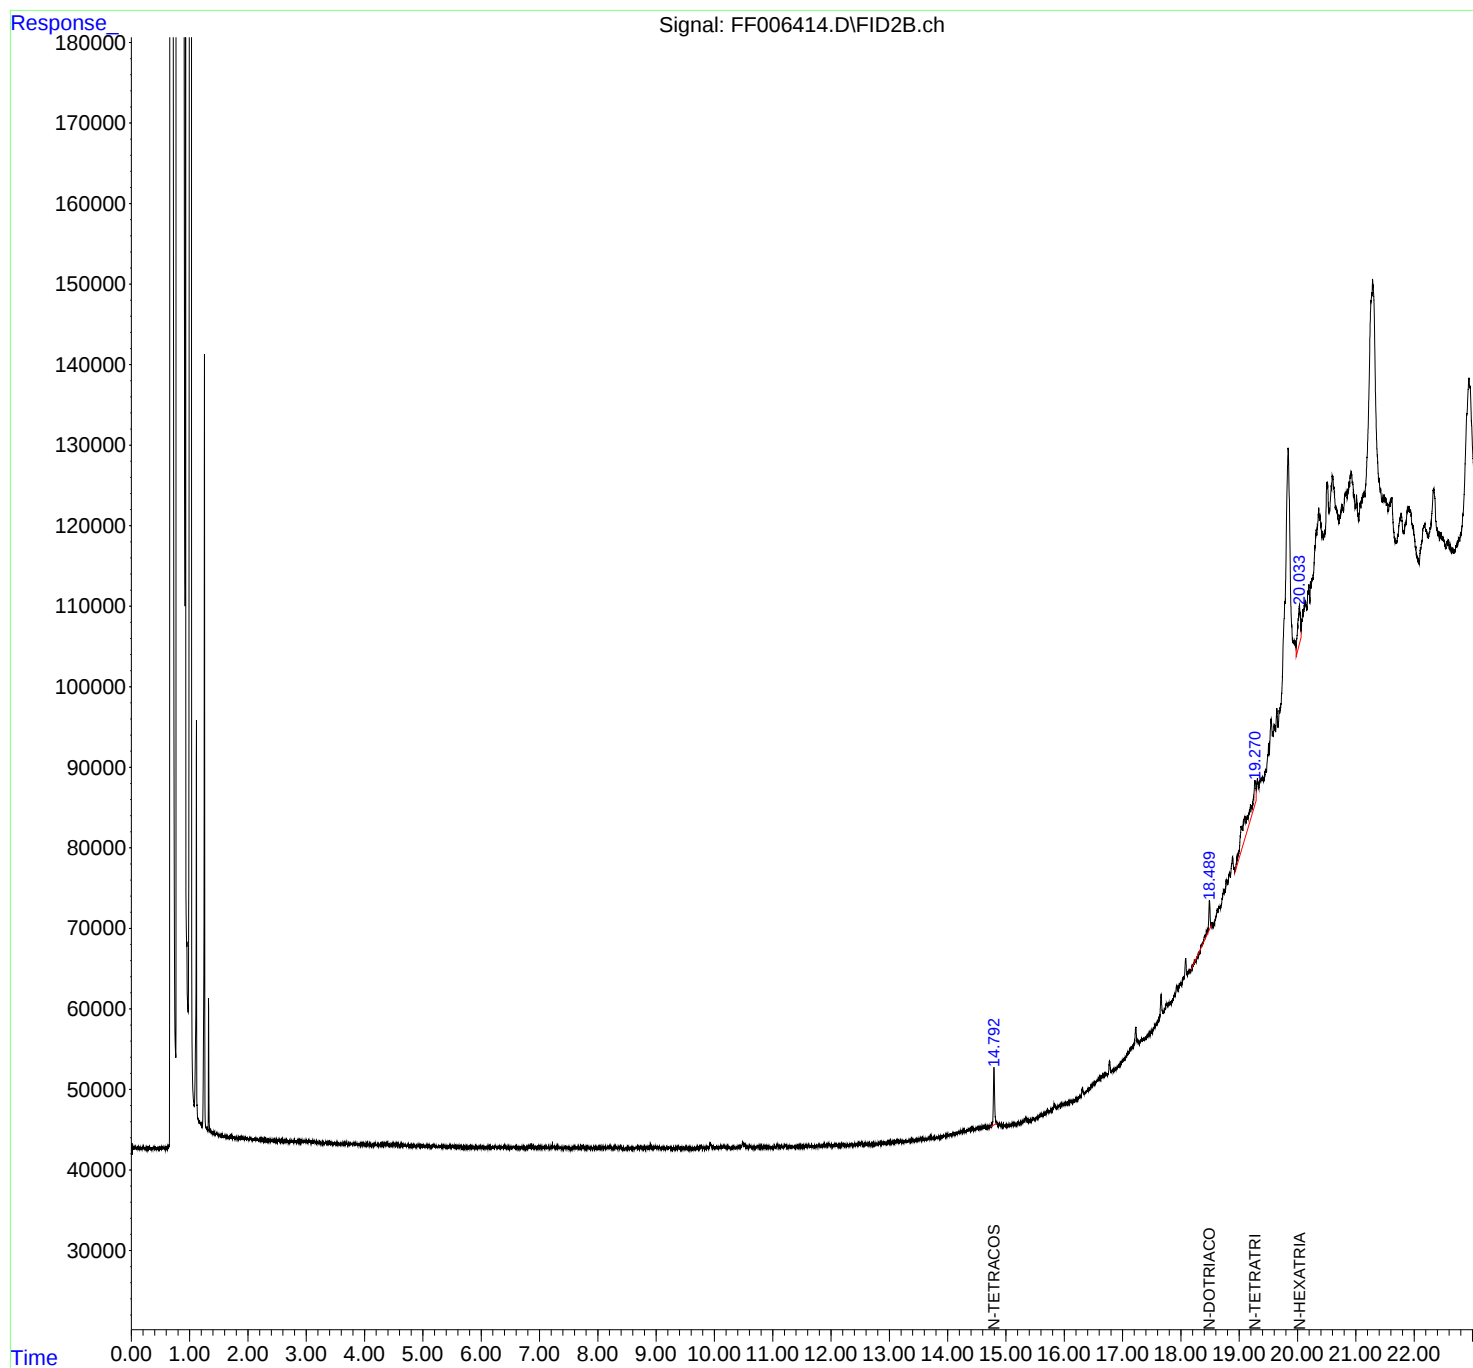


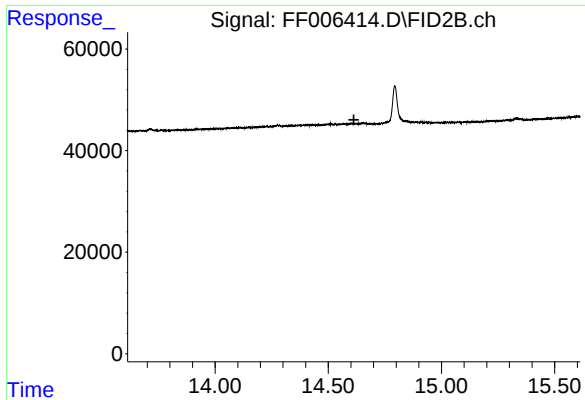

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.613 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

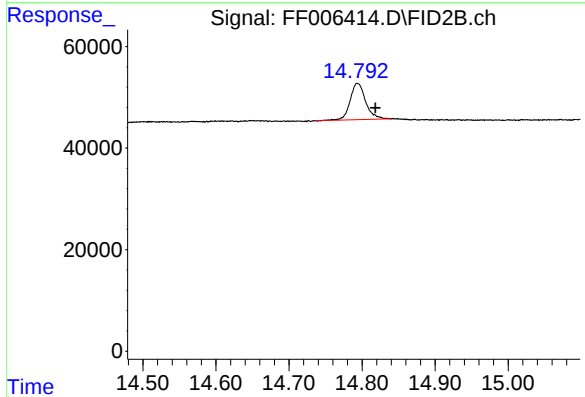


#10 N-TETRACOSANE

R.T.: 14.794 min
Delta R.T.: -0.024 min
Response: 105679
Conc: 0.76 ug/ml

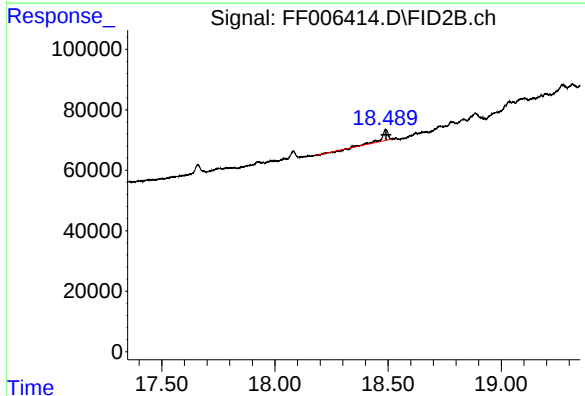


#14 N-DOTRIACONTANE

R.T.: 18.490 min
Delta R.T.: -0.002 min
Response: 64222
Conc: 0.49 ug/ml

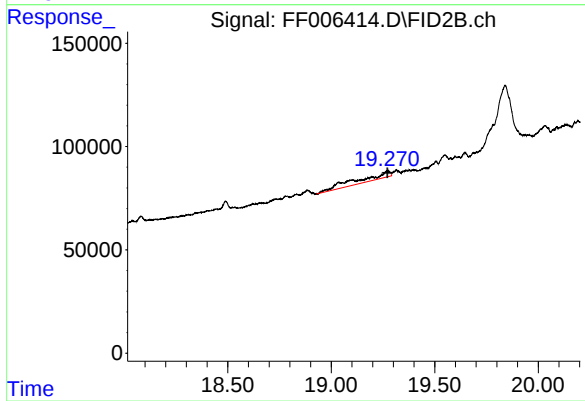

#15 N-TETRATRIACONTANE

R.T.: 19.269 min
Delta R.T.: -0.002 min
Response: 351344
Conc: 3.13 ug/ml

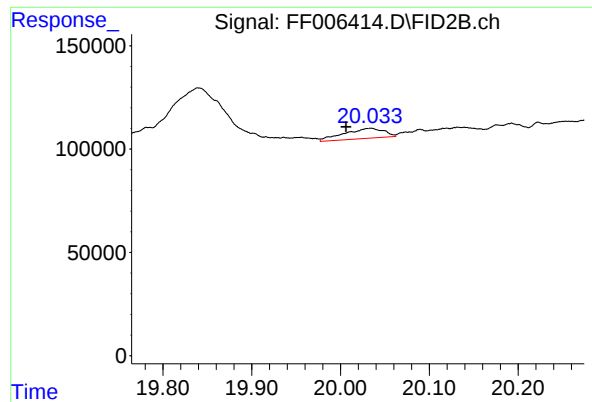

#16 N-HEXATRIACONTANE

R.T.: 20.034 min
Delta R.T.: 0.028 min
Response: 151532
Conc: 1.57 ug/ml

Instrument :
FID_F
ClientSampleId :