

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
Data File : FF006415.D
Signal(s) : FID2B.ch
Acq On : 17 Feb 2020 09:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 18 00:26:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.610	2024137	16.615 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.794	95227	0.681 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
Data File : FF006415.D
Signal(s) : FID2B.ch
Acq On : 17 Feb 2020 09:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 18 00:26:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

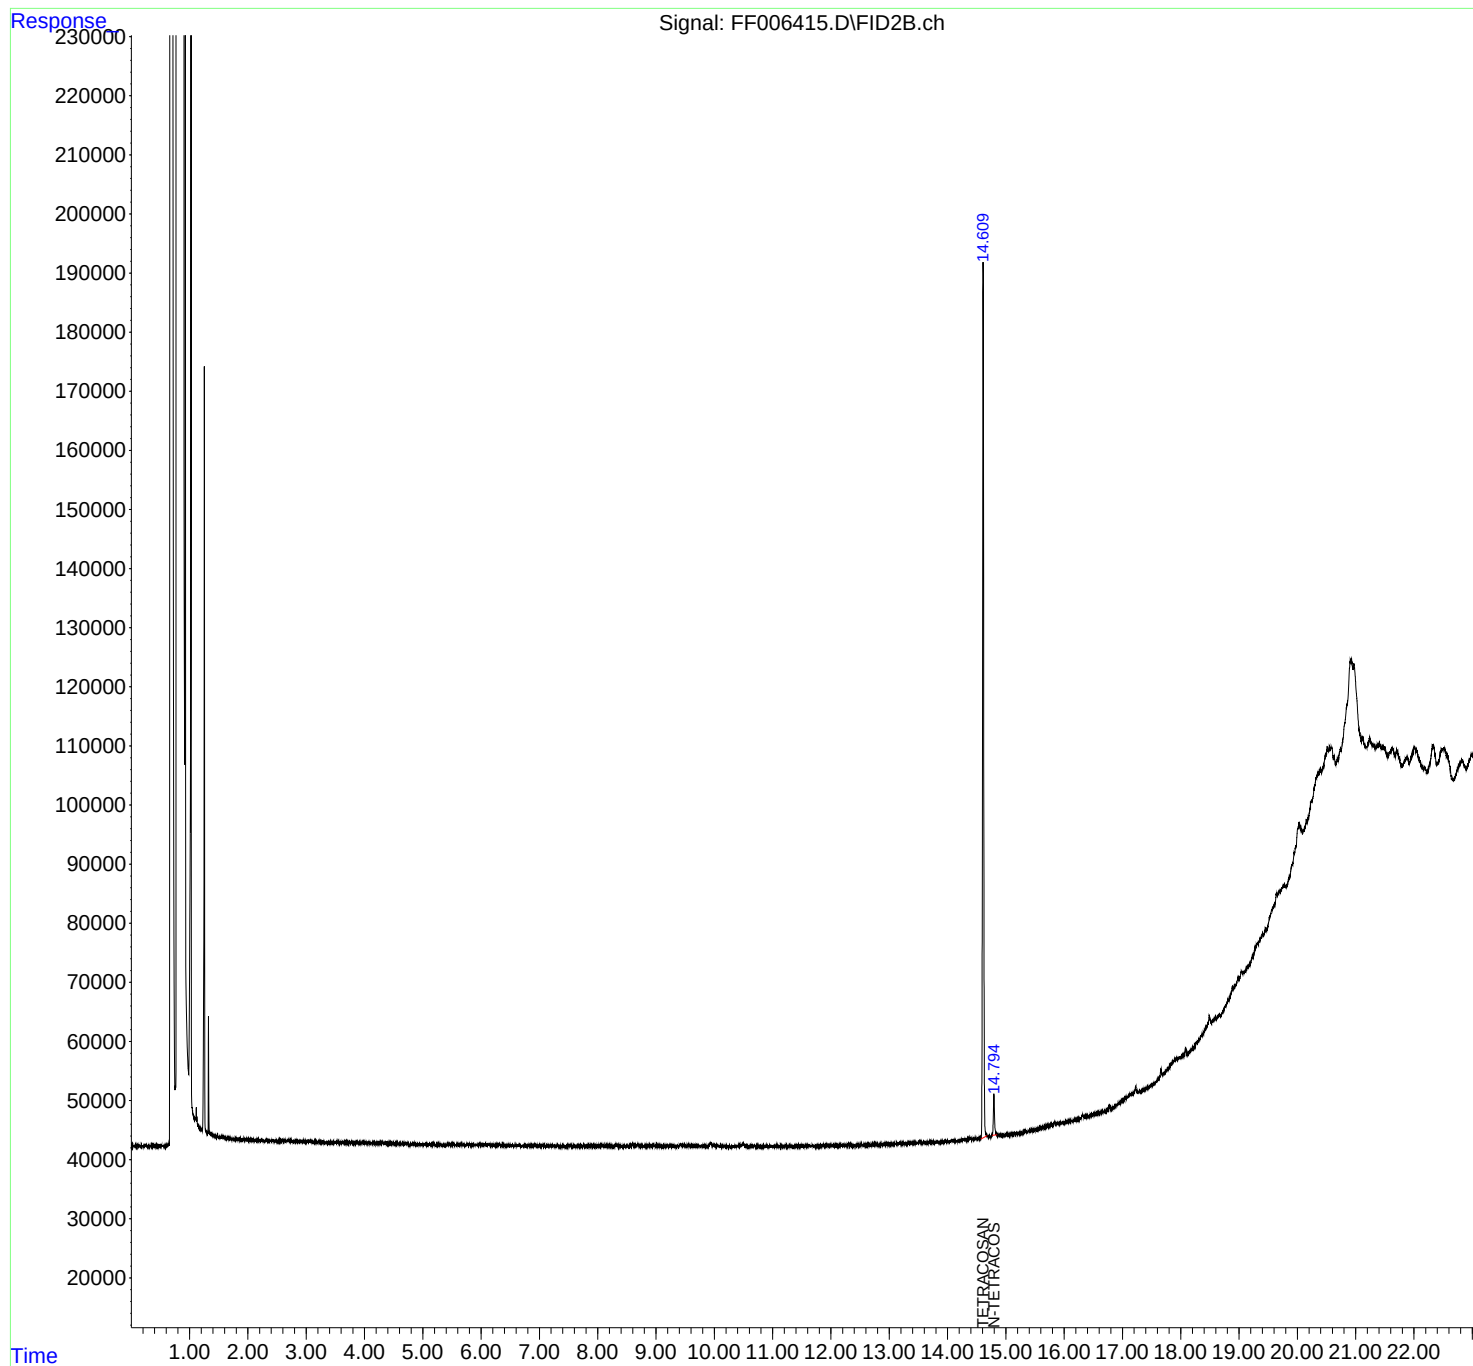


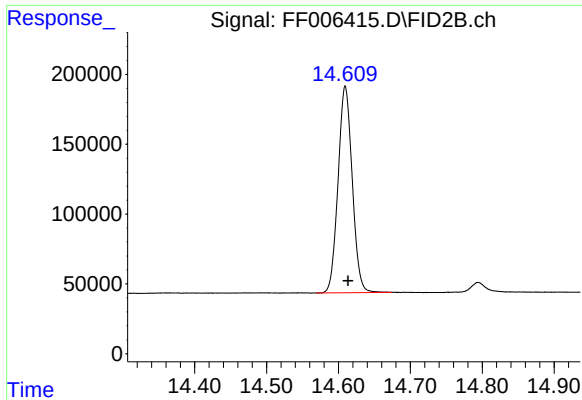

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.610 min
Delta R.T.: -0.004 min
Response: 2024137
Conc: 16.61 ug/ml

Instrument :
FID_F
ClientSampleId :

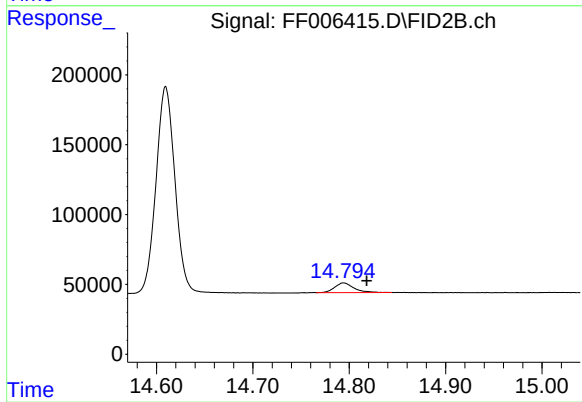

#10 N-TETRACOSANE

R.T.: 14.794 min
Delta R.T.: -0.024 min
Response: 95227
Conc: 0.68 ug/ml