

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
Data File : FF006417.D
Signal(s) : FID2B.ch
Acq On : 17 Feb 2020 10:25
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 18 00:27:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.390	2778358	20.329 ug/ml
10)	N-TETRACOSANE	14.794	106445	0.762 ug/ml
12)	N-OCTACOSANE	16.776	2711977	19.651 ug/ml
13)	N-TRIACONTANE	17.658	88157	0.637 ug/ml
16)	N-HEXATRIACONTANE	20.007	61484	0.635 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
Data File : FF006417.D
Signal(s) : FID2B.ch
Acq On : 17 Feb 2020 10:25
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 18 00:27:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

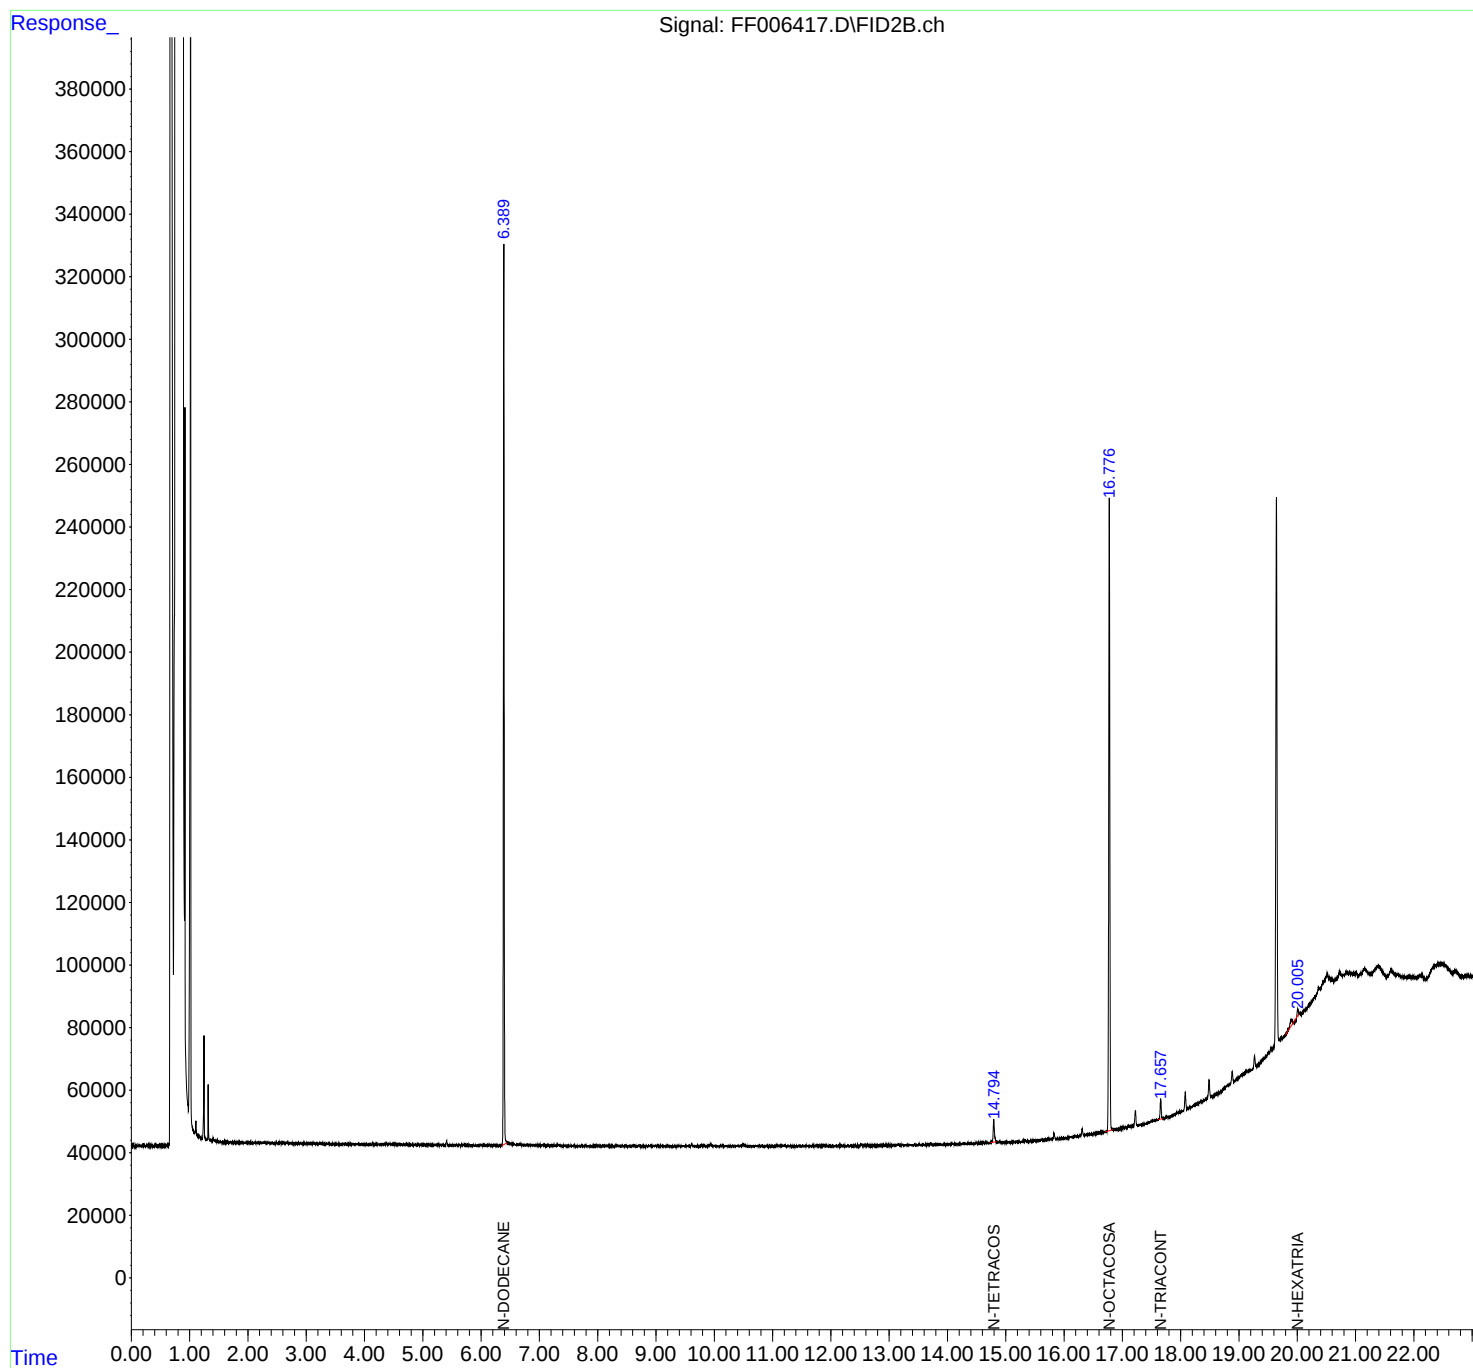


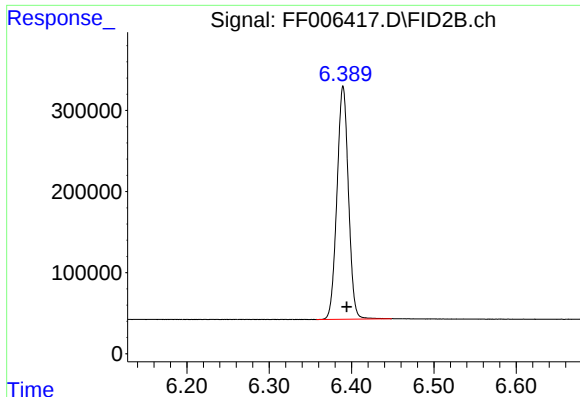

#3 N-DODECANE


R.T.: 6.390 min
Delta R.T.: -0.005 min
Response: 2778358
Conc: 20.33 ug/ml

Instrument :
FID_F
ClientSampleId :

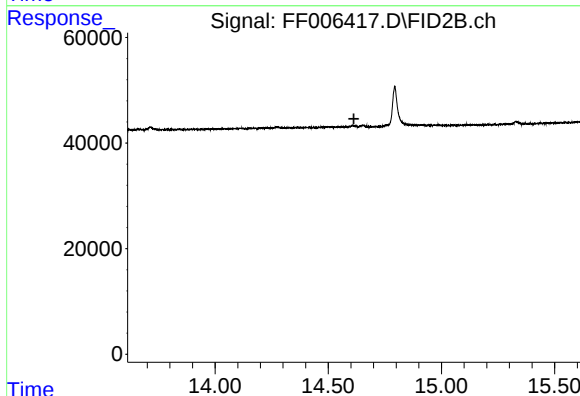


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.613 min
Response: 0
Conc: N.D.

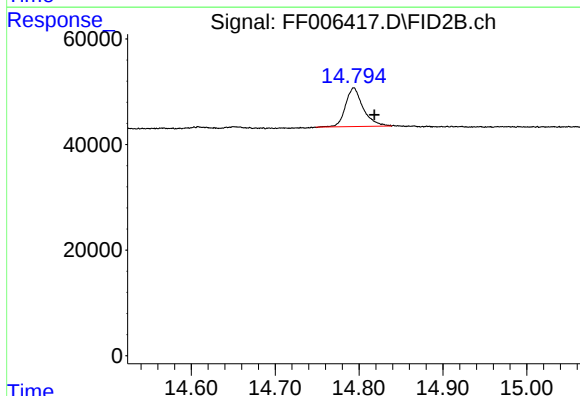


#10 N-TETRACOSANE

R.T.: 14.794 min
Delta R.T.: -0.024 min
Response: 106445
Conc: 0.76 ug/ml

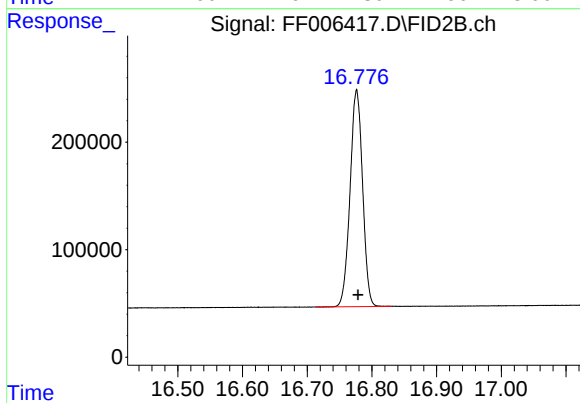

#12 N-OCTACOSANE


R.T.: 16.776 min
Delta R.T.: -0.002 min
Response: 2711977
Conc: 19.65 ug/ml

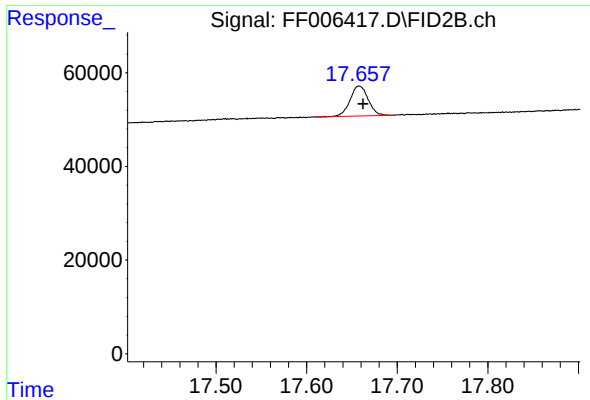

#13 N-TRIACONTANE

R.T.: 17.658 min
Delta R.T.: -0.004 min
Response: 88157
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

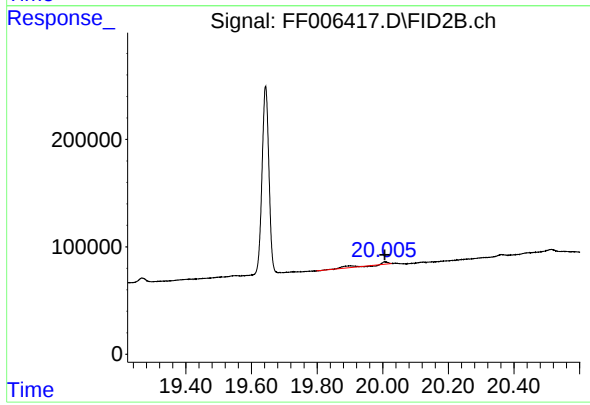

#16 N-HEXATRIACONTANE

R.T.: 20.007 min
Delta R.T.: 0.000 min
Response: 61484
Conc: 0.64 ug/ml