

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
 Data File : FF006420.D
 Signal(s) : FID2B.ch
 Acq On : 17 Feb 2020 11:55
 Operator : DD\AJ
 Sample : L1512-01 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 18 00:27:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	476671	3.913 ug/ml
Target Compounds			
7) N-EICOSANE	12.503	127542	0.905 ug/ml
8) N-DOCOSANE	13.745	252670	1.798 ug/ml
10) N-TETRACOSANE	14.796	1034305	7.402 ug/ml
12) N-OCTACOSANE	16.791	263694	1.911 ug/ml
13) N-TRIACONTANE	17.658	213065	1.541 ug/ml
14) N-DOTRIACONTANE	18.444	92221	0.701 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
 Data File : FF006420.D
 Signal(s) : FID2B.ch
 Acq On : 17 Feb 2020 11:55
 Operator : DD\AJ
 Sample : L1512-01 5X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 18 00:27:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

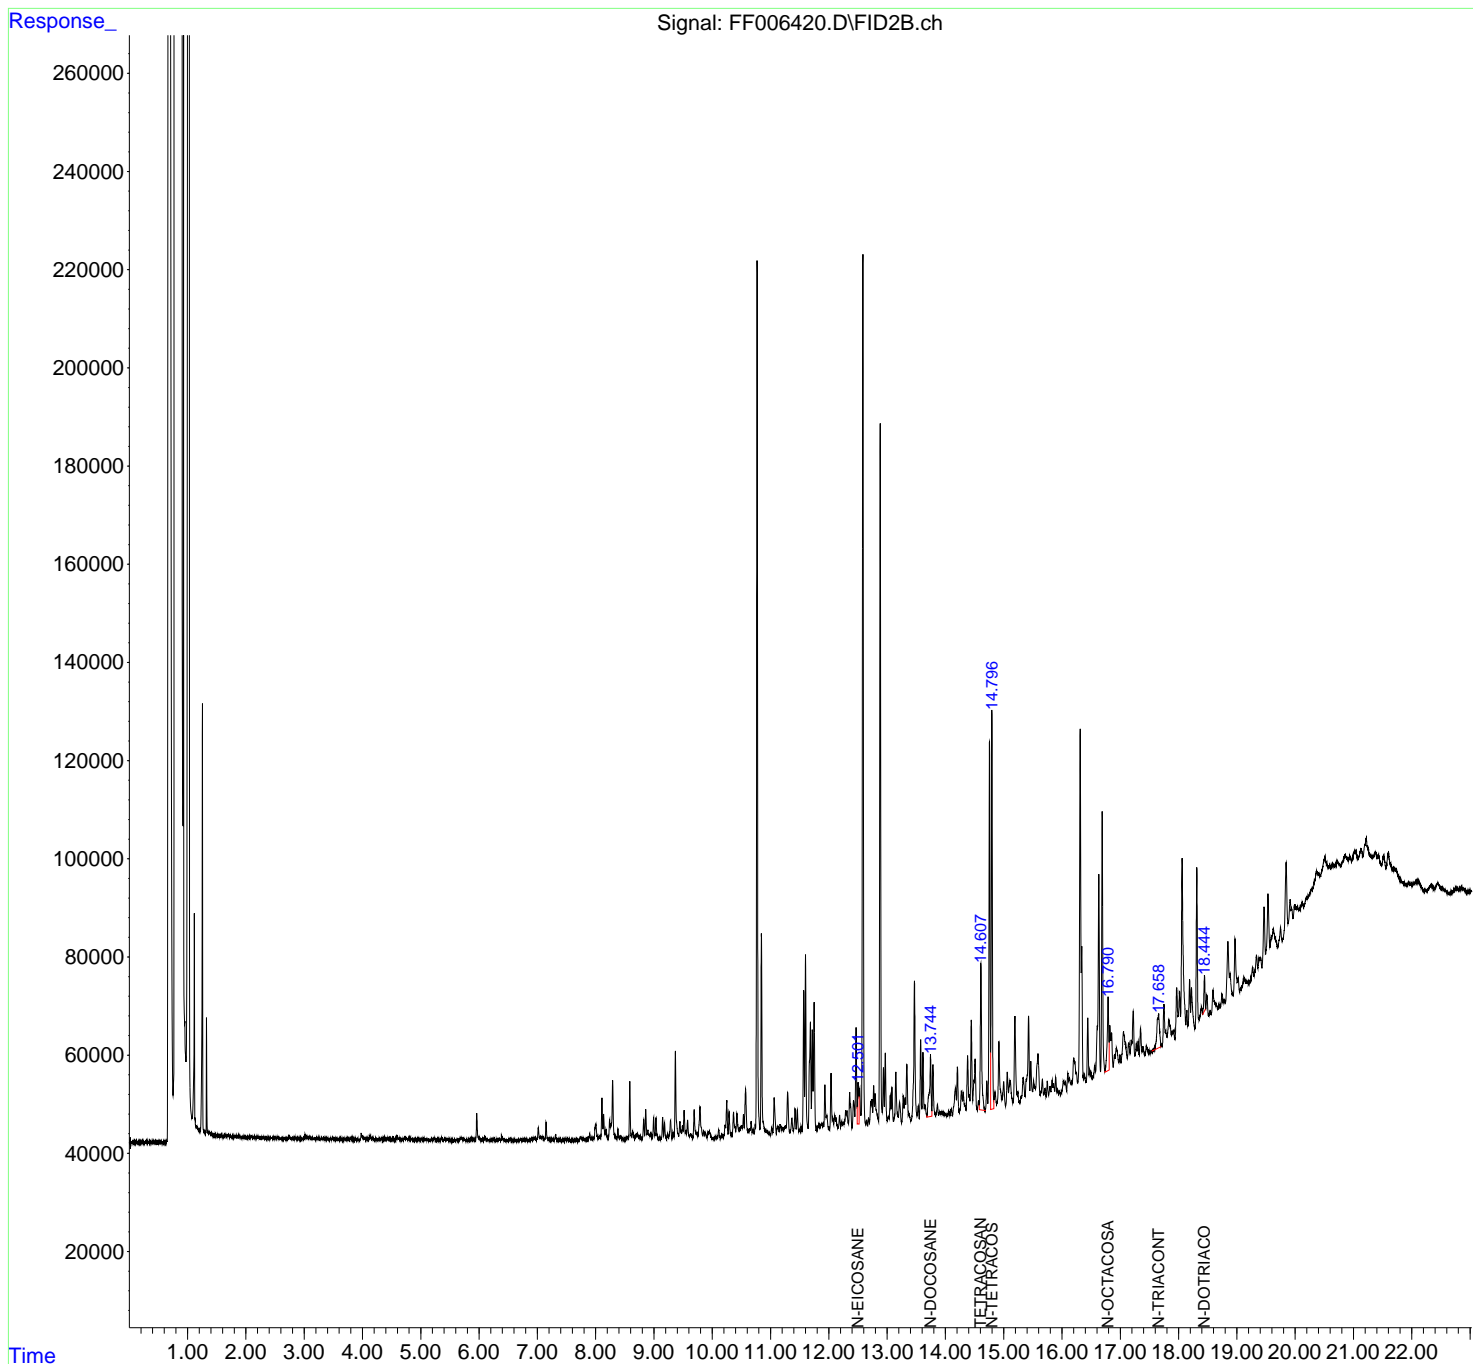


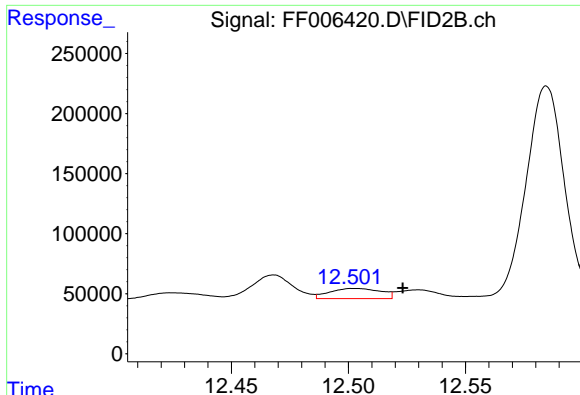

#7 N-EICOSANE


R.T.: 12.503 min
 Delta R.T.: -0.021 min
 Response: 127542
 Conc: 0.90 ug/ml

Instrument :
 FID_F
 ClientSampled :

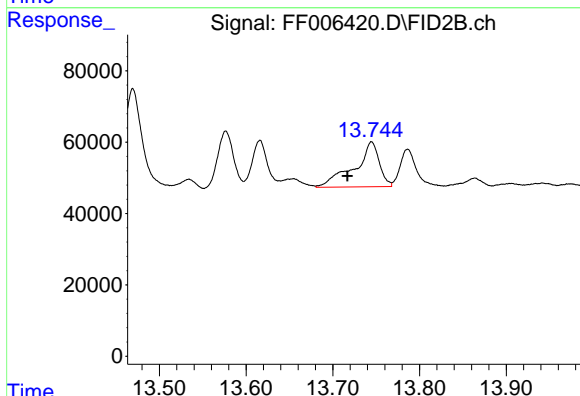


#8 N-DOCOSANE

R.T.: 13.745 min
 Delta R.T.: 0.028 min
 Response: 252670
 Conc: 1.80 ug/ml

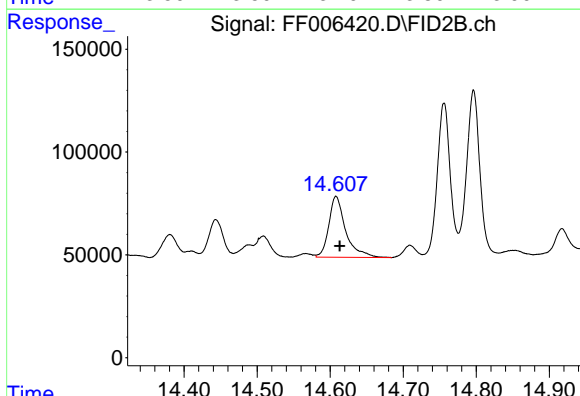


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.608 min
 Delta R.T.: -0.005 min
 Response: 476671
 Conc: 3.91 ug/ml

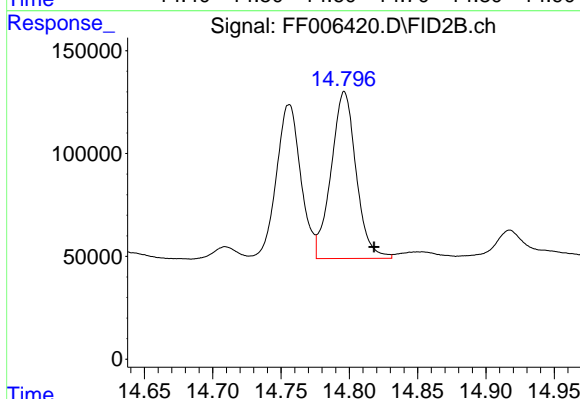


#10 N-TETRACOSANE

R.T.: 14.796 min
 Delta R.T.: -0.022 min
 Response: 1034305
 Conc: 7.40 ug/ml

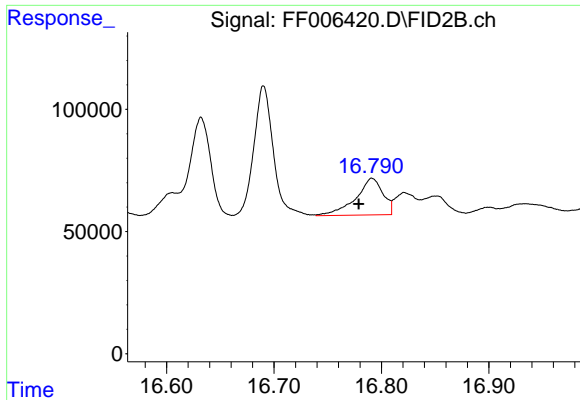


#12 N-OCTACOSANE
 R.T.: 16.791 min
 Delta R.T.: 0.012 min
 Response: 263694
 Conc: 1.91 ug/ml

Instrument :
 FID_F
 ClientSampleId :

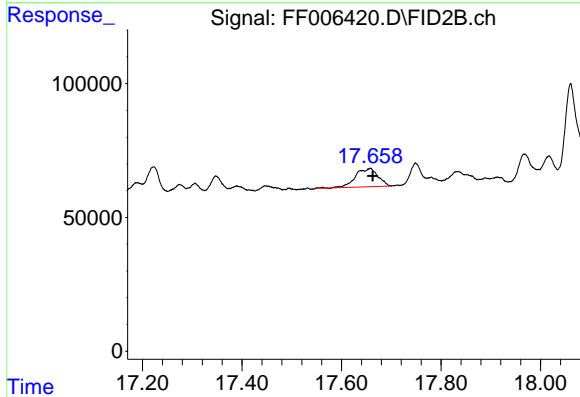

#13 N-TRIACONTANE
 R.T.: 17.658 min
 Delta R.T.: -0.004 min
 Response: 213065
 Conc: 1.54 ug/ml

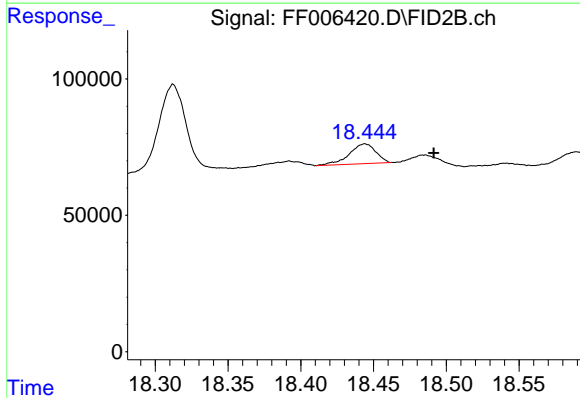

#14 N-DOTRIACONTANE
 R.T.: 18.444 min
 Delta R.T.: -0.047 min
 Response: 92221
 Conc: 0.70 ug/ml