

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
 Data File : FF006421.D
 Signal(s) : FID2B.ch
 Acq On : 17 Feb 2020 12:44
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 18 00:27:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	2117855	17.384 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.792	251884	1.803 ug/ml
14) N-DOTRIACONTANE	18.488	92244	0.701 ug/ml
16) N-HEXATRIACONTANE	20.035	65861	0.681 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF021720\
Data File : FF006421.D
Signal(s) : FID2B.ch
Acq On : 17 Feb 2020 12:44
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 18 00:27:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

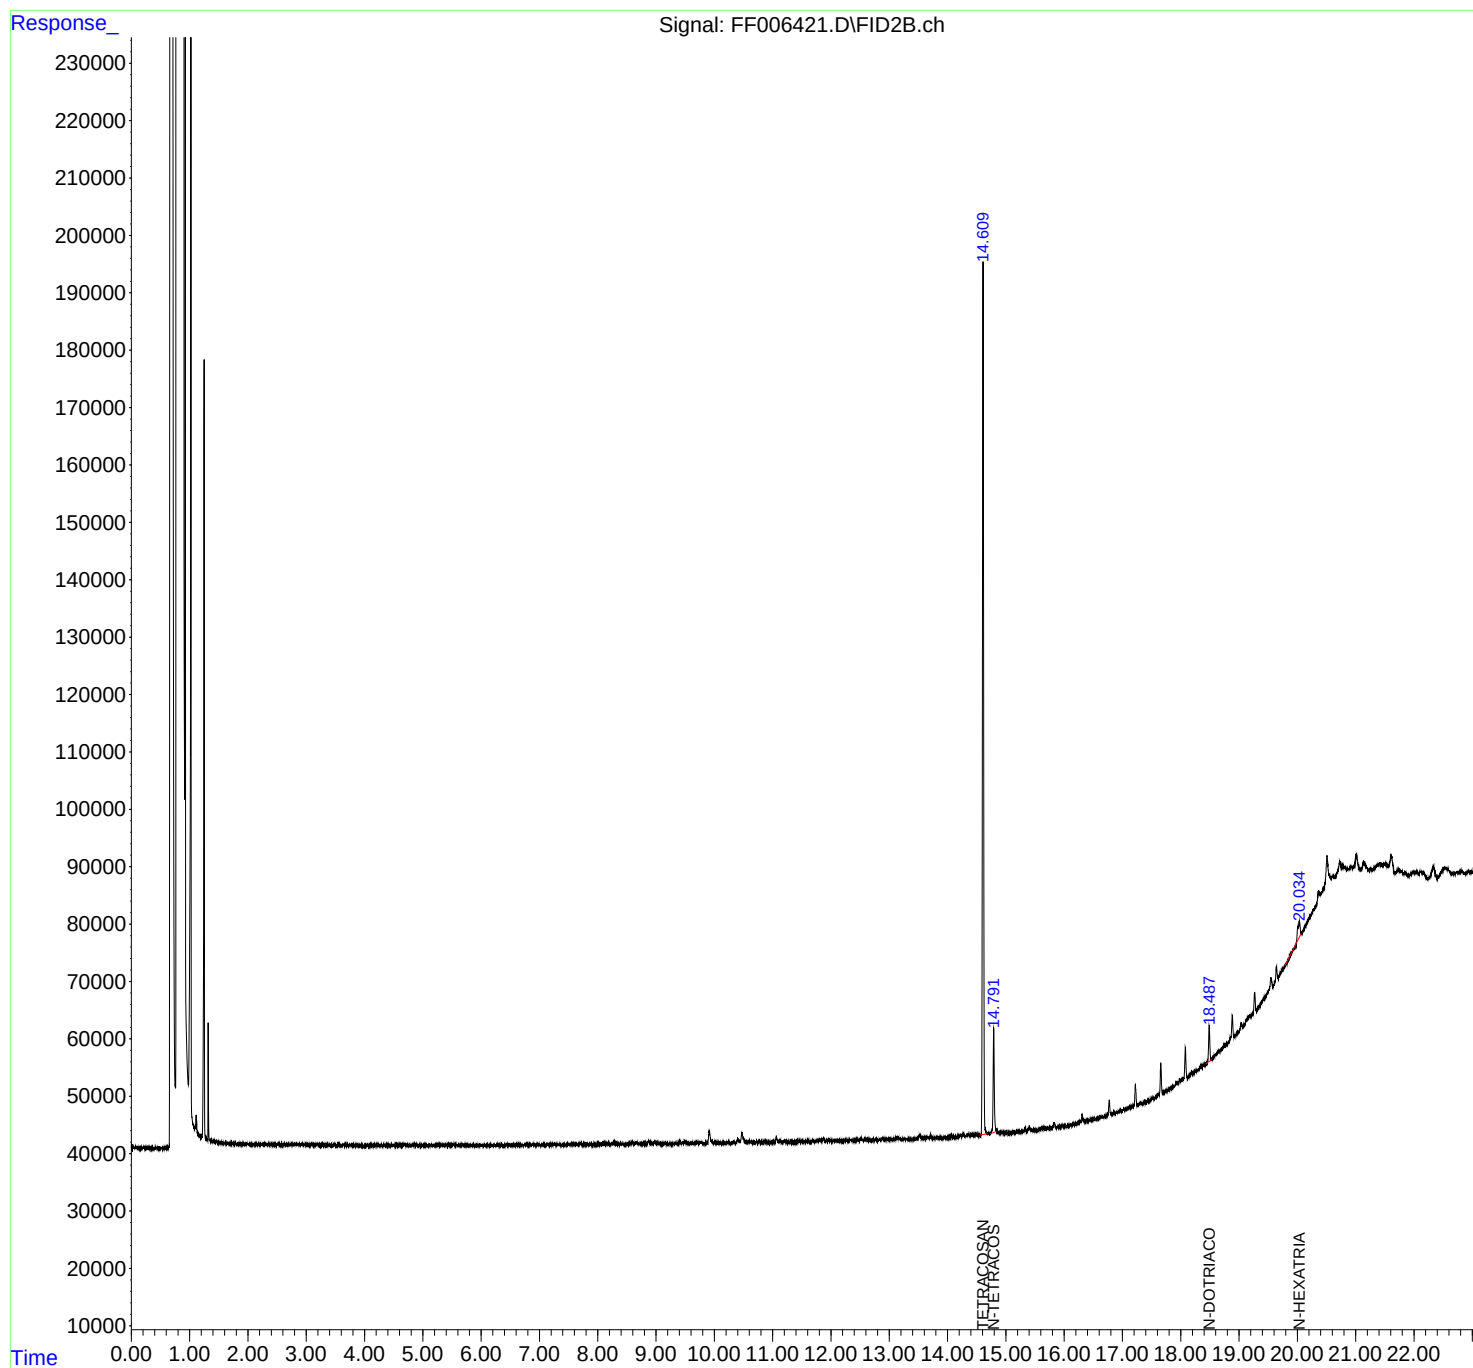


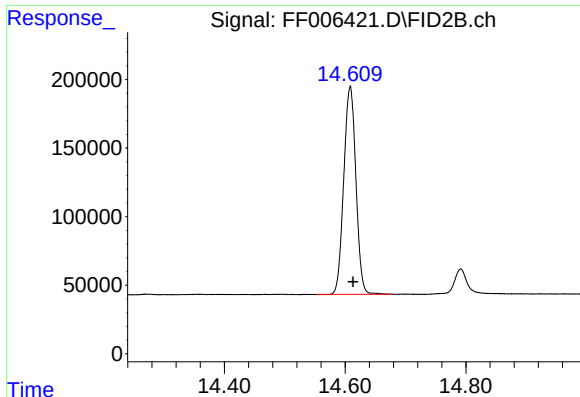

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.608 min
Delta R.T.: -0.005 min
Response: 2117855
Conc: 17.38 ug/ml

Instrument :
FID_F
ClientSampleId :

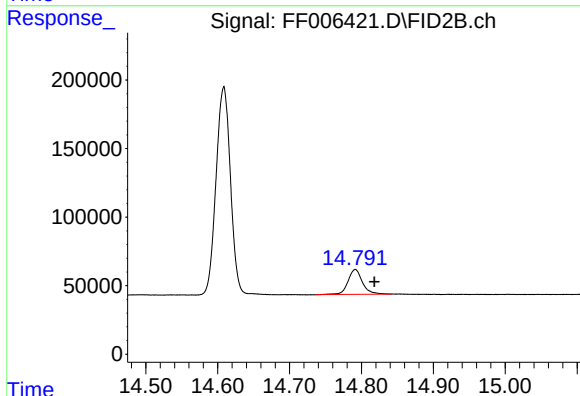


#10 N-TETRACOSANE

R.T.: 14.792 min
Delta R.T.: -0.027 min
Response: 251884
Conc: 1.80 ug/ml

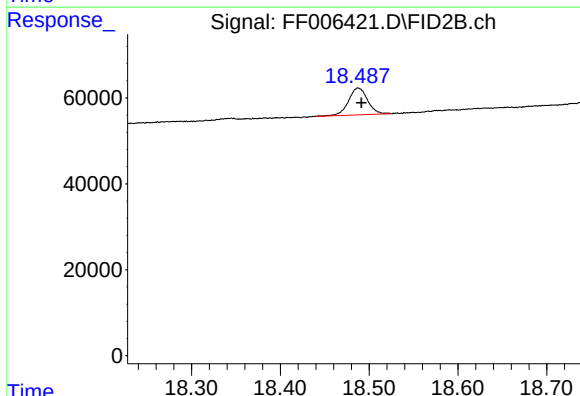

#14 N-DOTRIACONTANE

R.T.: 18.488 min
Delta R.T.: -0.004 min
Response: 92244
Conc: 0.70 ug/ml

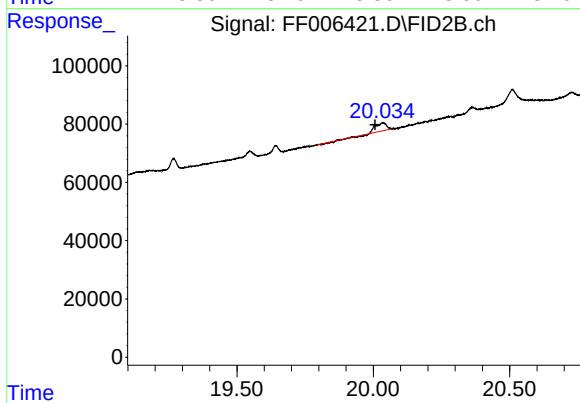

#16 N-HEXATRIACONTANE

R.T.: 20.035 min
Delta R.T.: 0.028 min
Response: 65861
Conc: 0.68 ug/ml