

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022020\
Data File : FF006432.D
Signal(s) : FID2B.ch
Acq On : 20 Feb 2020 16:11
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 00:31:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.605	2150332	17.650 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.789	105055	0.752 ug/ml
14) N-DOTRIACONTANE	18.484	100856	0.767 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022020\
Data File : FF006432.D
Signal(s) : FID2B.ch
Acq On : 20 Feb 2020 16:11
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 00:31:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

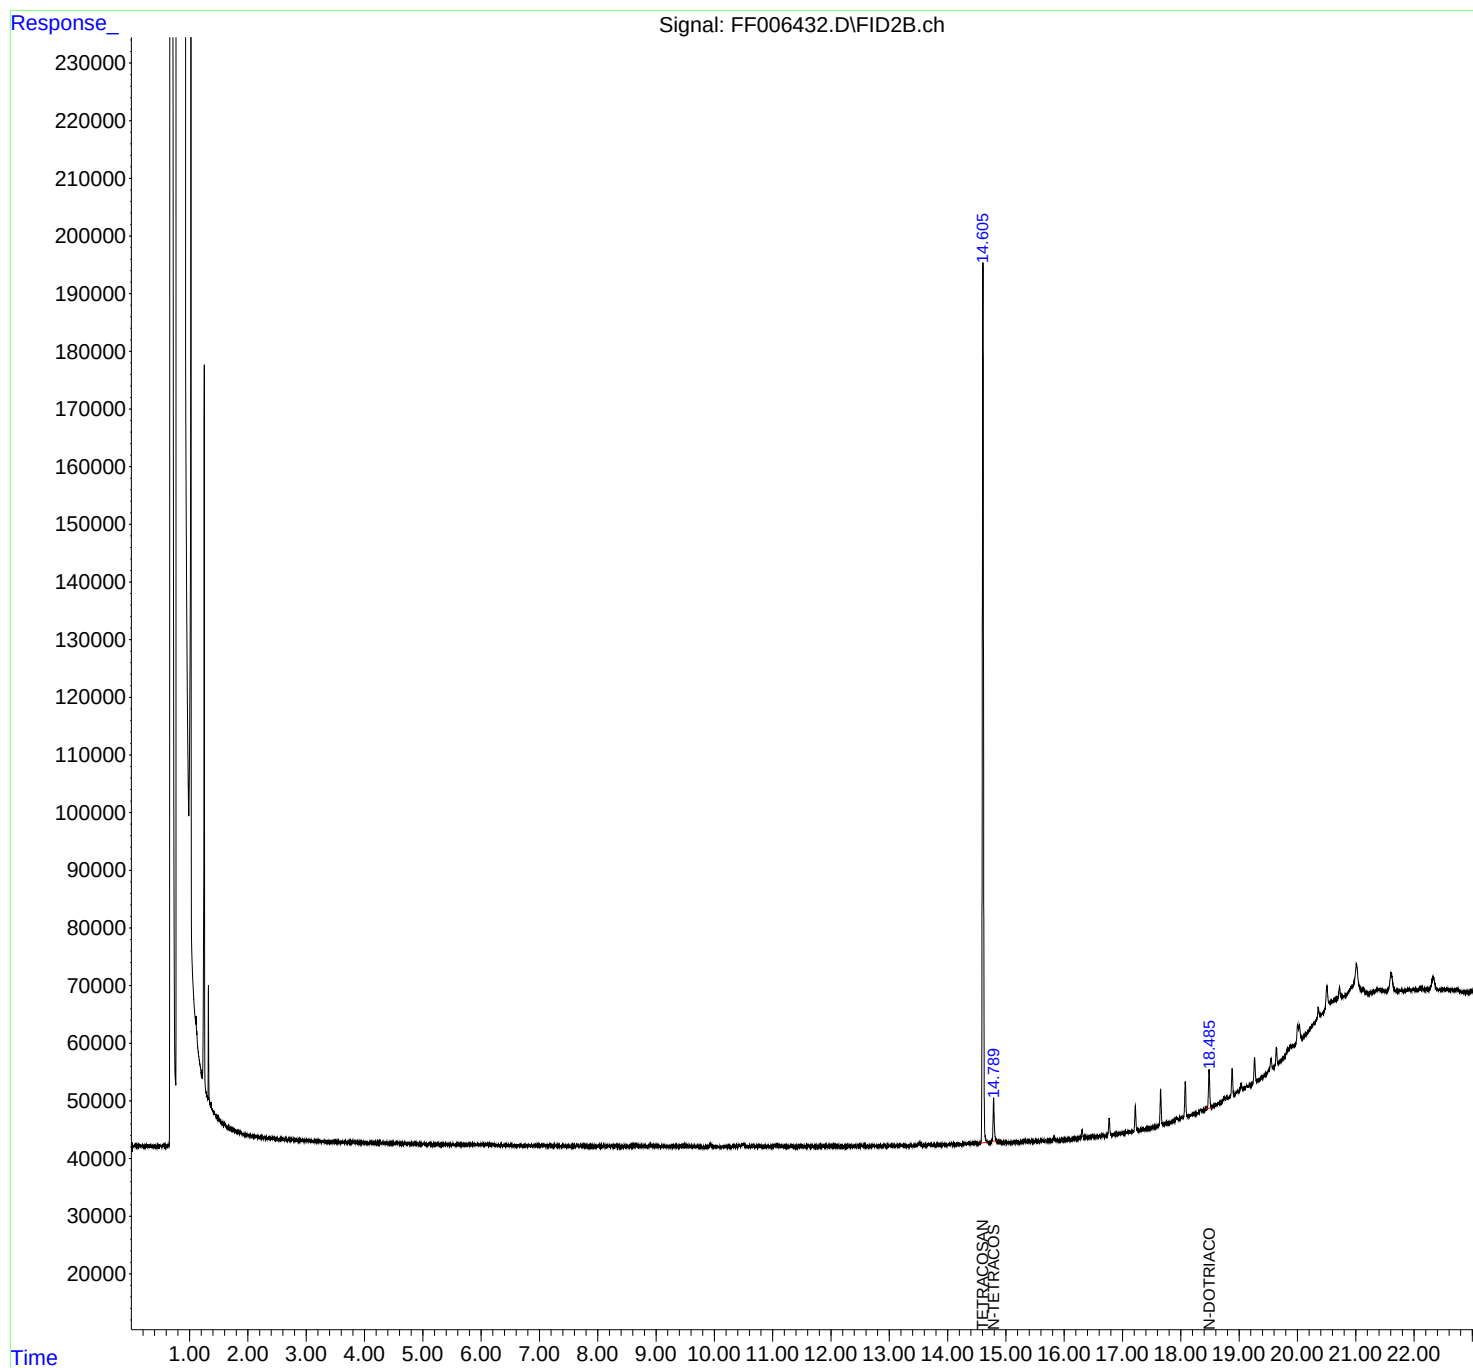

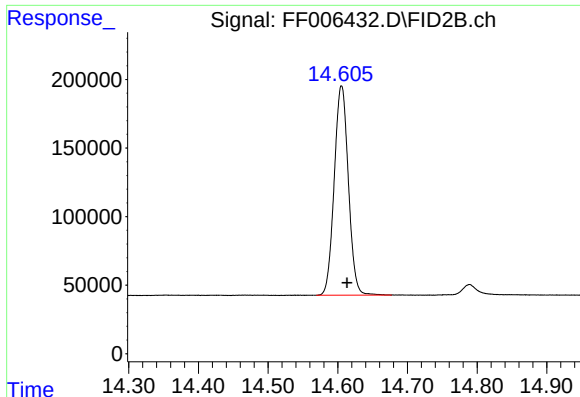


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.605 min
Delta R.T.: -0.008 min
Response: 2150332
Conc: 17.65 ug/ml

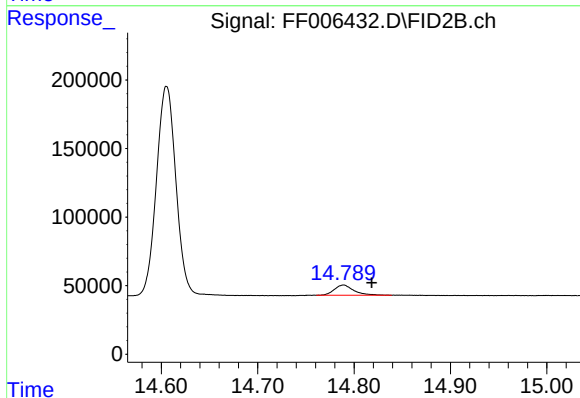

#10 N-TETRACOSANE

R.T.: 14.789 min
Delta R.T.: -0.029 min
Response: 105055
Conc: 0.75 ug/ml

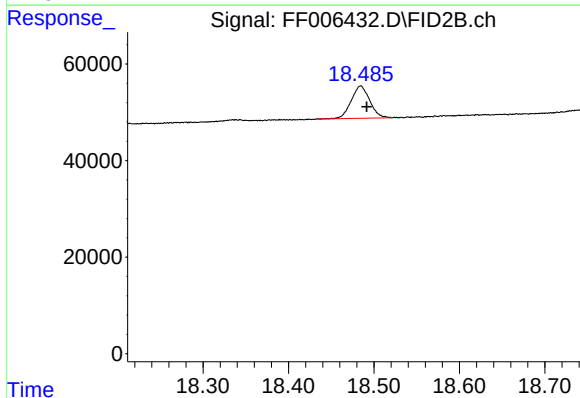

#14 N-DOTRIACONTANE

R.T.: 18.484 min
Delta R.T.: -0.007 min
Response: 100856
Conc: 0.77 ug/ml