

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022119\
 Data File : FF003577.D
 Signal(s) : FID2B.ch
 Acq On : 21 Feb 2019 09:55
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 21 23:50:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.603	2182771	18.080 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.783	88908	0.649 ug/ml
13) N-TRIACONTANE	17.675	171216	1.213 ug/ml
14) N-DOTRIACONTANE	18.513	248489	1.801 ug/ml
15) N-TETRATRIACONTANE	19.298	138710	1.094 ug/ml
16) N-HEXATRIACONTANE	20.044	93000	0.796 ug/ml
18) N-TETRACONTANE	21.696	373425	3.449 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022119\
Data File : FF003577.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2019 09:55
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 23:50:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

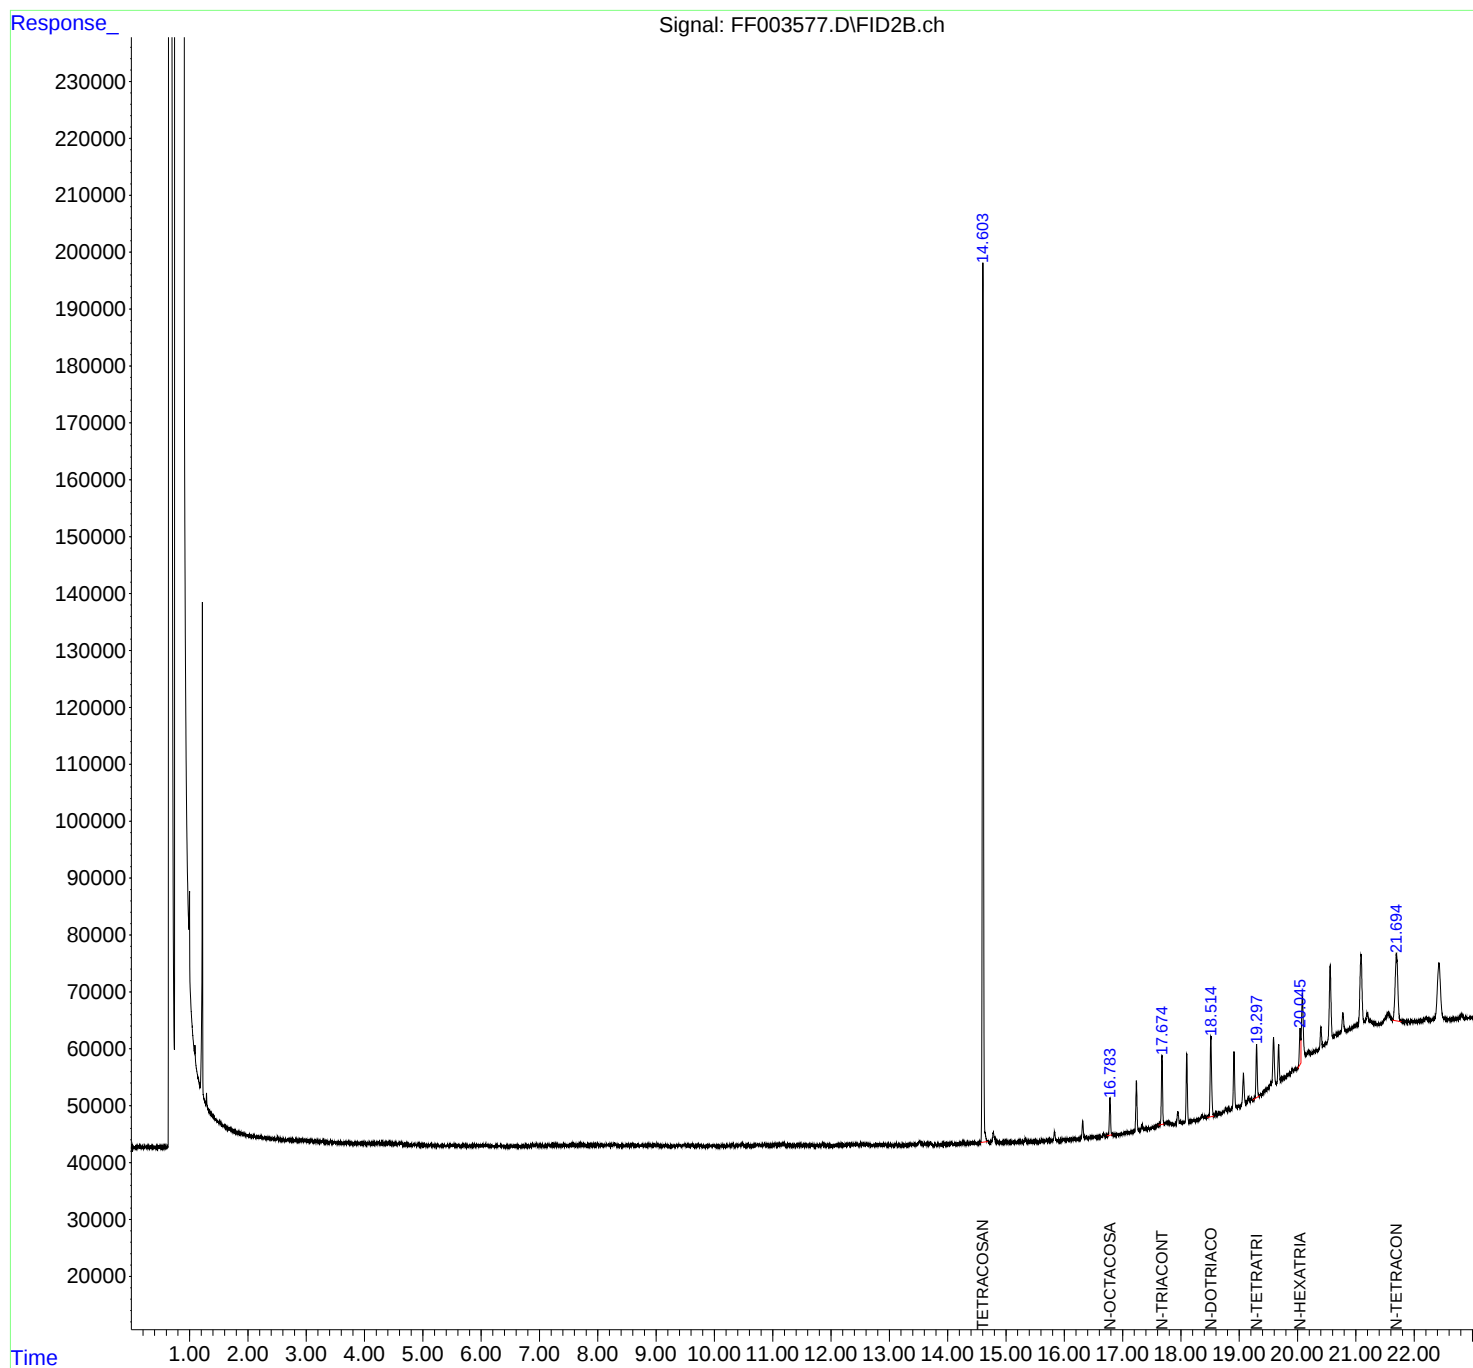

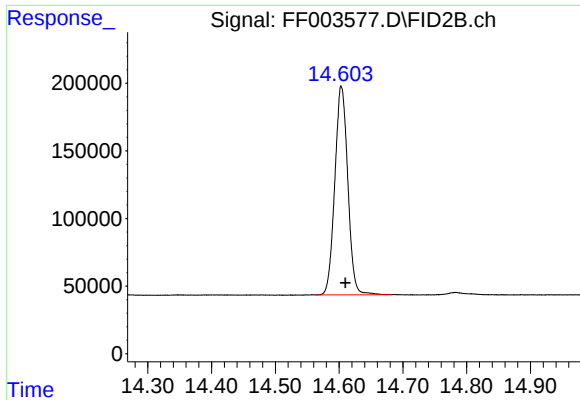


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.603 min
Delta R.T.: -0.007 min
Response: 2182771
Conc: 18.08 ug/ml

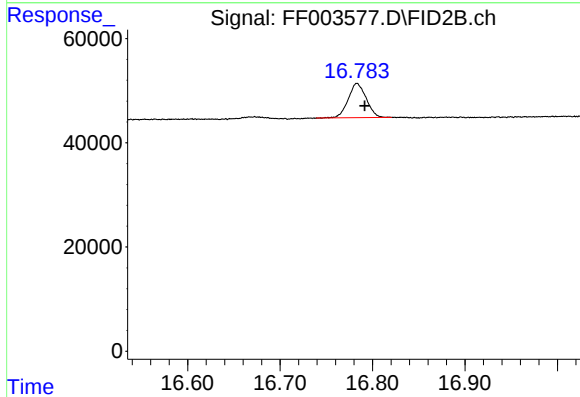


#12 N-OCTACOSANE

R.T.: 16.783 min
Delta R.T.: -0.008 min
Response: 88908
Conc: 0.65 ug/ml

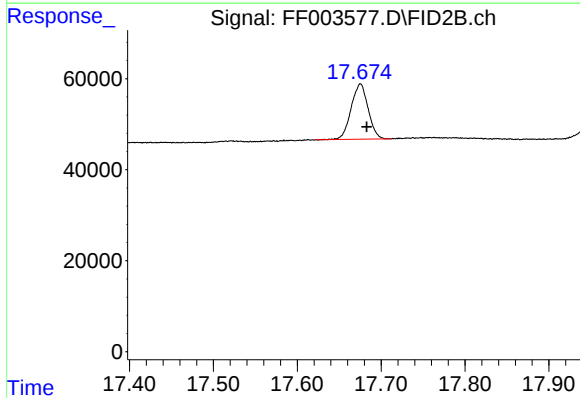


#13 N-TRIACONTANE

R.T.: 17.675 min
Delta R.T.: -0.008 min
Response: 171216
Conc: 1.21 ug/ml

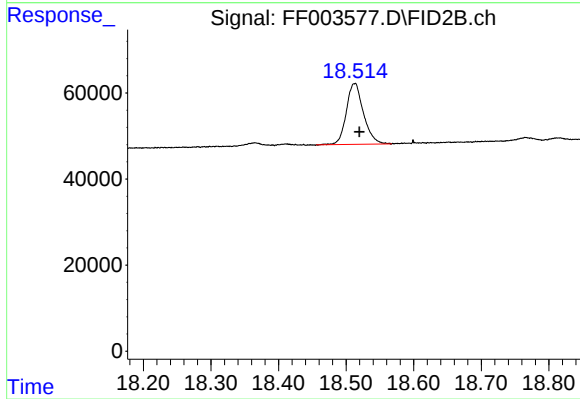


#14 N-DOTRIACONTANE

R.T.: 18.513 min
Delta R.T.: -0.007 min
Response: 248489
Conc: 1.80 ug/ml

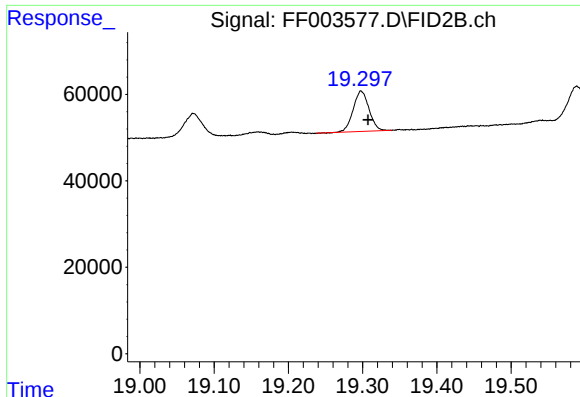


#15 N-TETRATRIACONTANE

R.T.: 19.298 min
Delta R.T.: -0.009 min
Response: 138710
Conc: 1.09 ug/ml

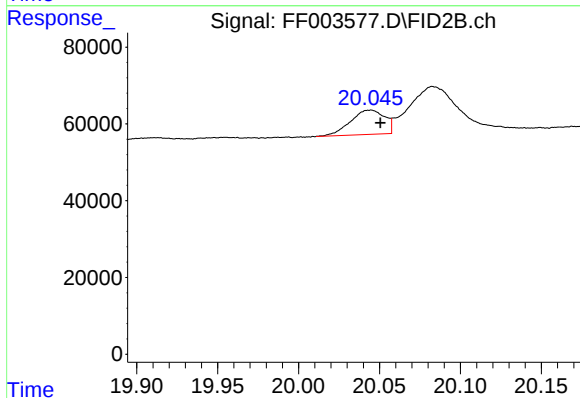

#16 N-HEXATRIACONTANE

R.T.: 20.044 min
Delta R.T.: -0.006 min
Response: 93000
Conc: 0.80 ug/ml

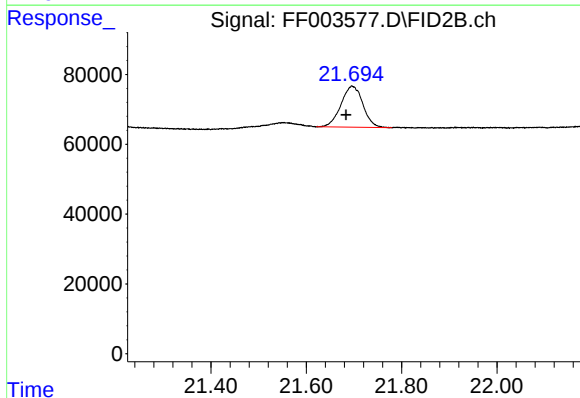

#18 N-TETRACONTANE

R.T.: 21.696 min
Delta R.T.: 0.013 min
Response: 373425
Conc: 3.45 ug/ml