

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022119\
Data File : FF003579.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2019 11:01
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 23:51:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.350	2879912	21.360 ug/ml
12)	N-OCTACOSANE	16.788	2675958	19.545 ug/ml
13)	N-TRIACONTANE	17.677	163379	1.157 ug/ml
14)	N-DOTRIACONTANE	18.514	182850	1.325 ug/ml
15)	N-TETRATRIACONTANE	19.301	128789	1.015 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022119\
Data File : FF003579.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2019 11:01
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 23:51:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

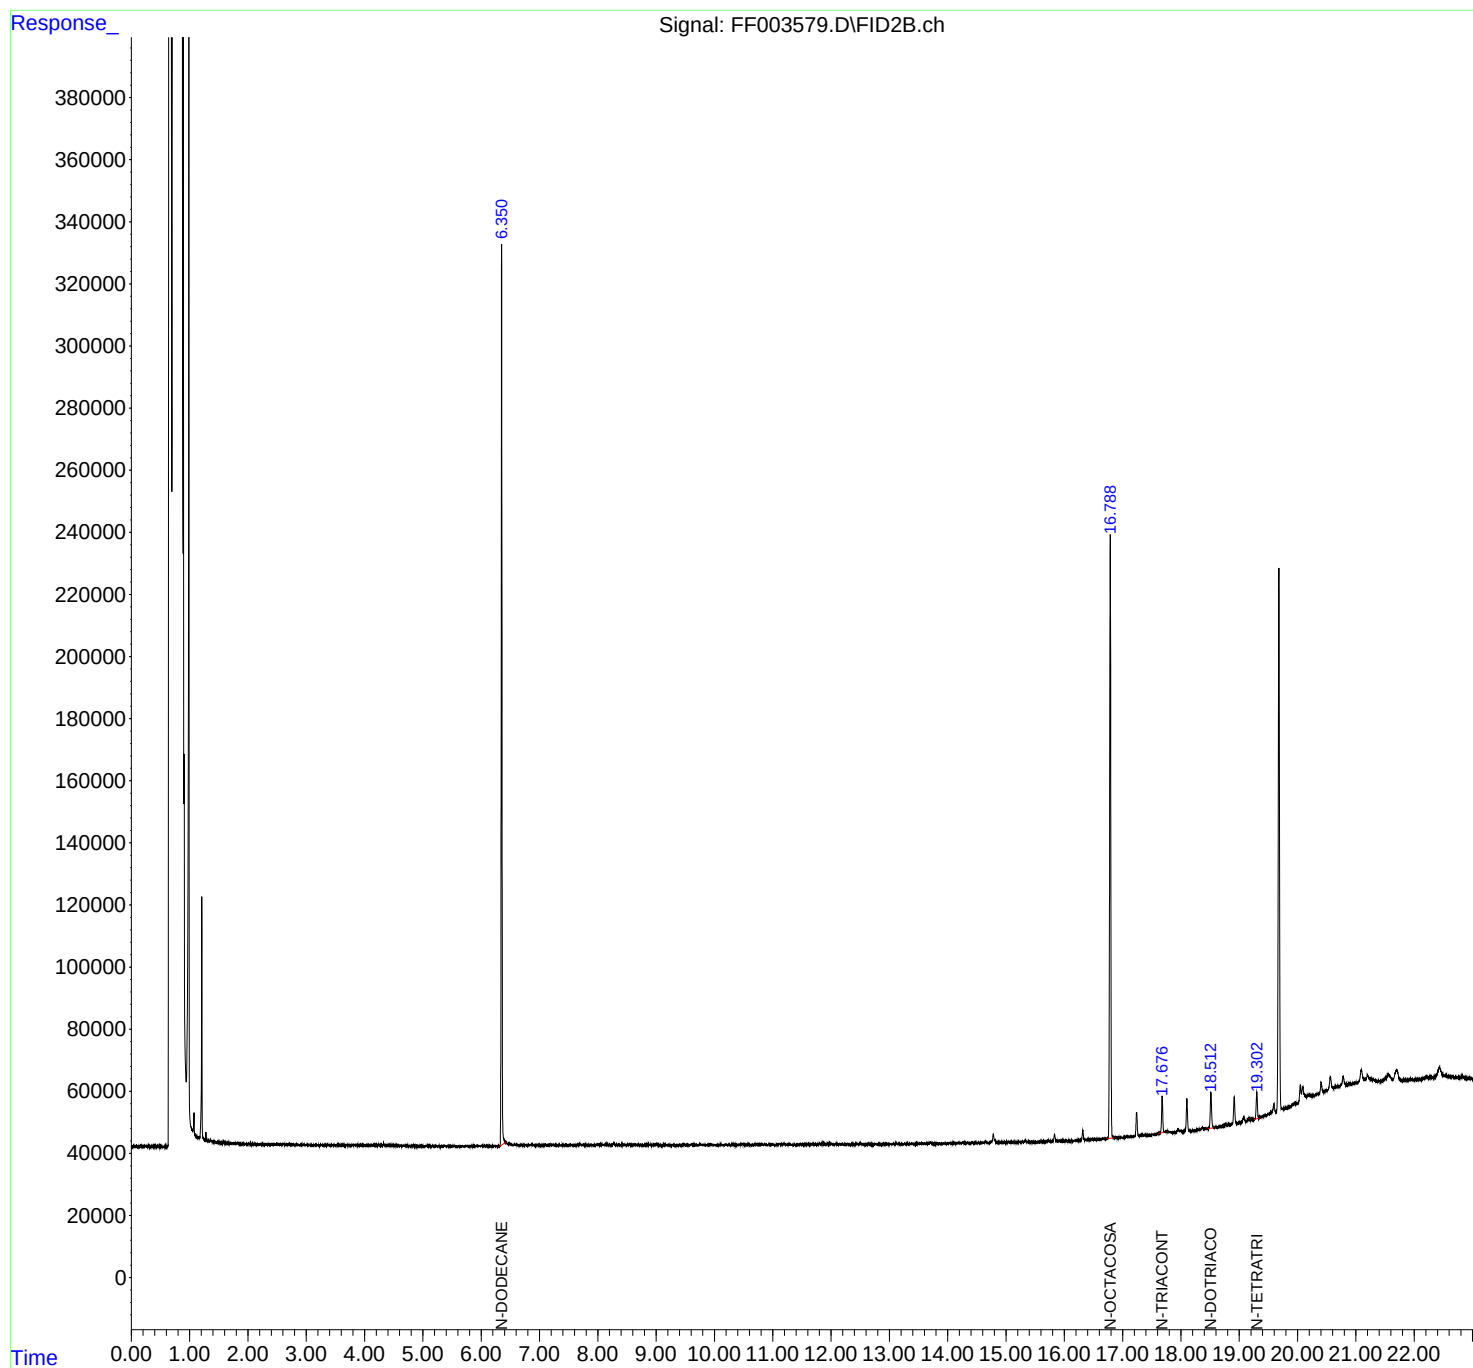

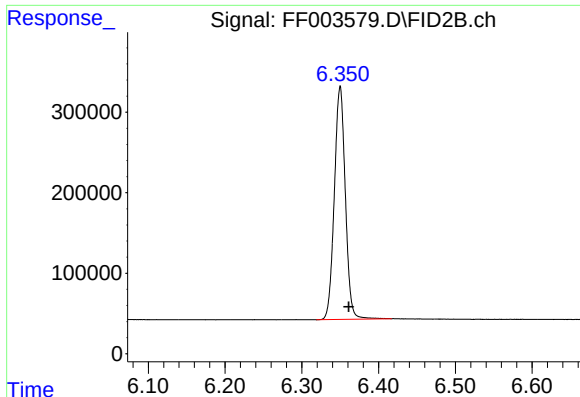


#3 N-DODECANE

R.T.: 6.350 min
Delta R.T.: -0.011 min
Response: 2879912
Conc: 21.36 ug/ml

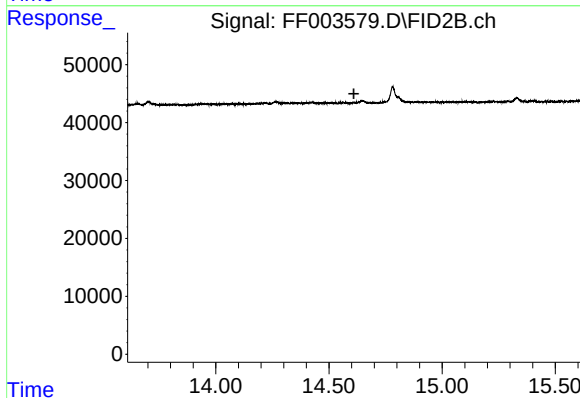


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.610 min
Response: 0
Conc: N.D.

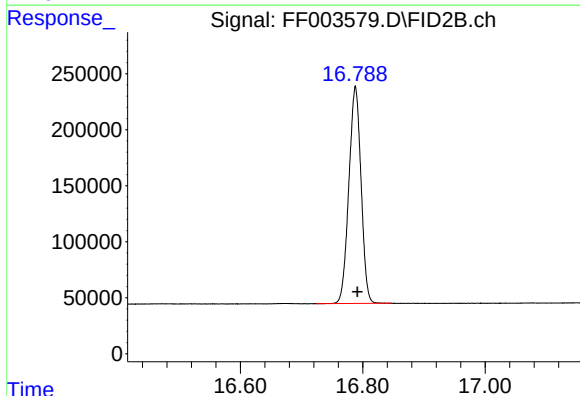


#12 N-OCTACOSANE

R.T.: 16.788 min
Delta R.T.: -0.003 min
Response: 2675958
Conc: 19.54 ug/ml

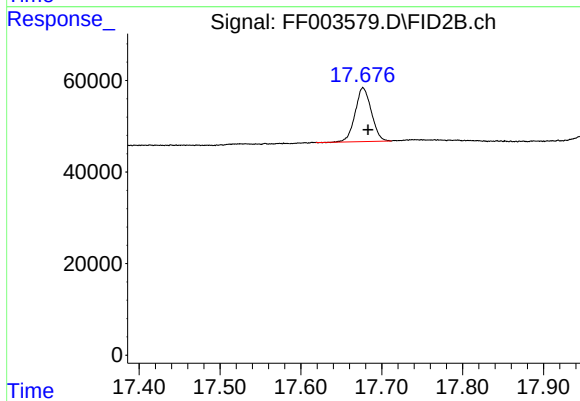


#13 N-TRIACONTANE

R.T.: 17.677 min
Delta R.T.: -0.006 min
Response: 163379
Conc: 1.16 ug/ml

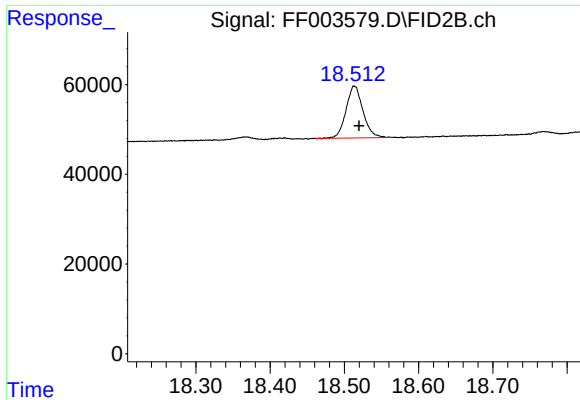

#14 N-DOTRIACONTANE

R.T.: 18.514 min
Delta R.T.: -0.006 min
Response: 182850
Conc: 1.32 ug/ml

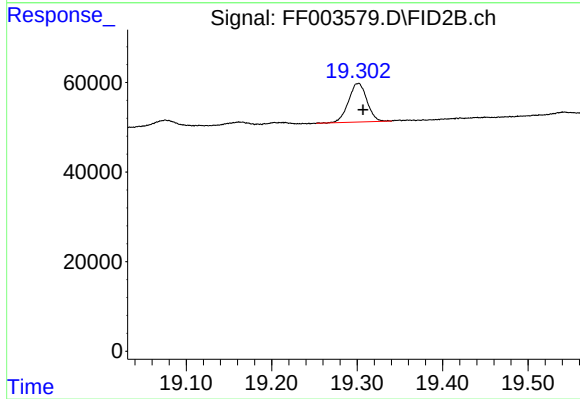

#15 N-TETRATRIACONTANE

R.T.: 19.301 min
Delta R.T.: -0.006 min
Response: 128789
Conc: 1.02 ug/ml