

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022119\
Data File : FF003580.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2019 12:28
Operator : AJ\SJ
Sample : PB117261BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 23:51:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.603	2223633	18.419 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.779	146983	1.081 ug/ml
12) N-OCTACOSANE	16.786	96962	0.708 ug/ml
13) N-TRIACONTANE	17.677	179098	1.268 ug/ml
14) N-DOTRIACONTANE	18.514	218101	1.580 ug/ml
15) N-TETRATRIACONTANE	19.304	147700	1.164 ug/ml
16) N-HEXATRIACONTANE	20.051	71799	0.614 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022119\
Data File : FF003580.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2019 12:28
Operator : AJ\SJ
Sample : PB117261BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 23:51:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

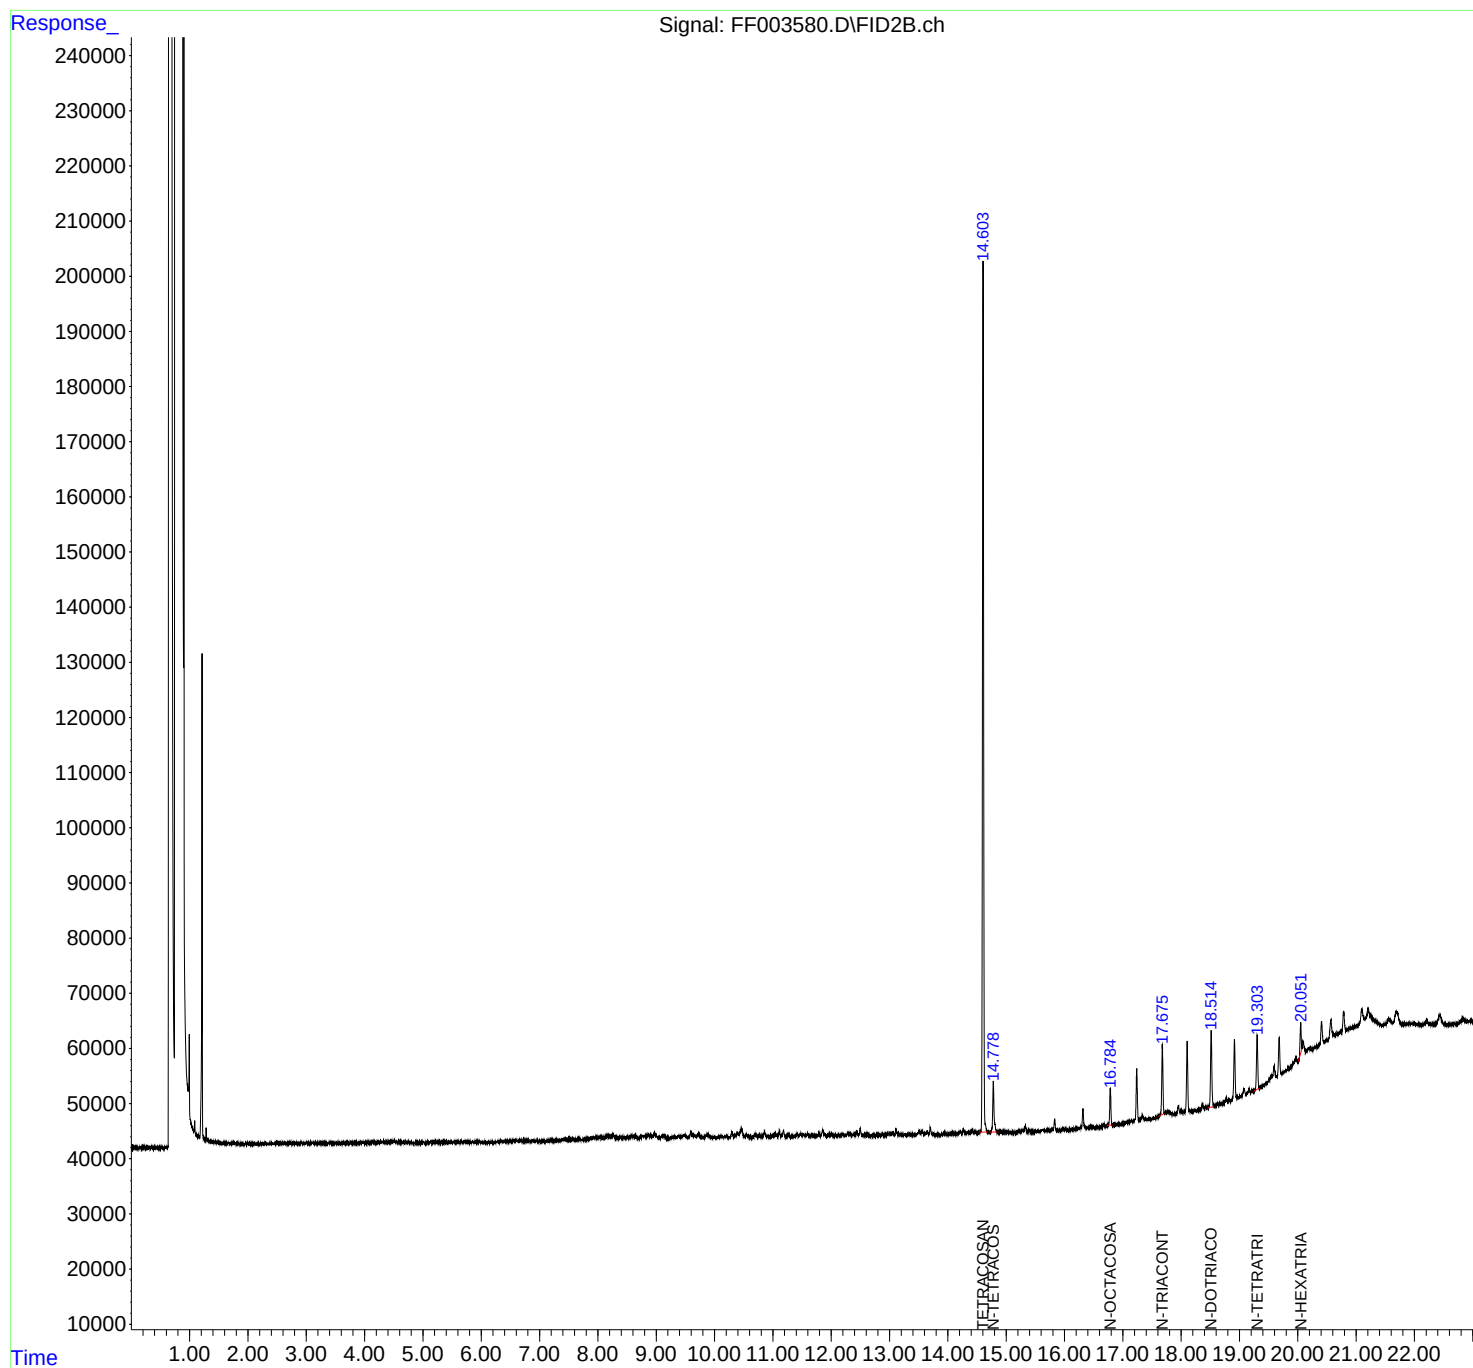

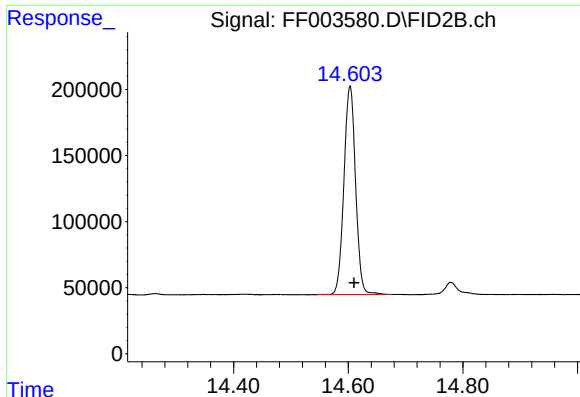


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.603 min
Delta R.T.: -0.007 min
Response: 2223633
Conc: 18.42 ug/ml

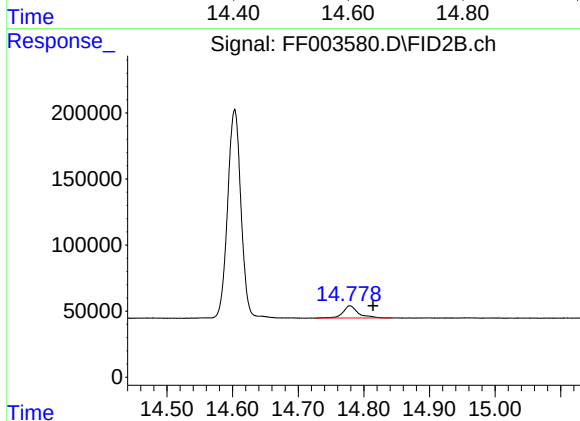


#10 N-TETRACOSANE

R.T.: 14.779 min
Delta R.T.: -0.035 min
Response: 146983
Conc: 1.08 ug/ml

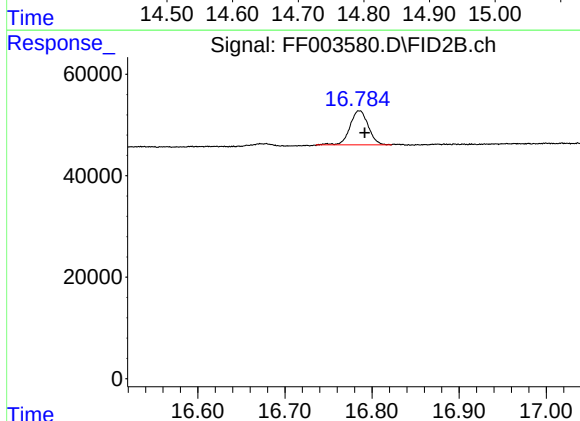


#12 N-OCTACOSANE

R.T.: 16.786 min
Delta R.T.: -0.006 min
Response: 96962
Conc: 0.71 ug/ml

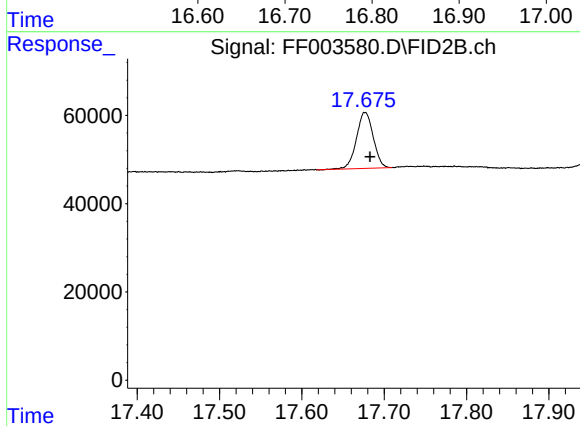


#13 N-TRIACONTANE

R.T.: 17.677 min
Delta R.T.: -0.006 min
Response: 179098
Conc: 1.27 ug/ml

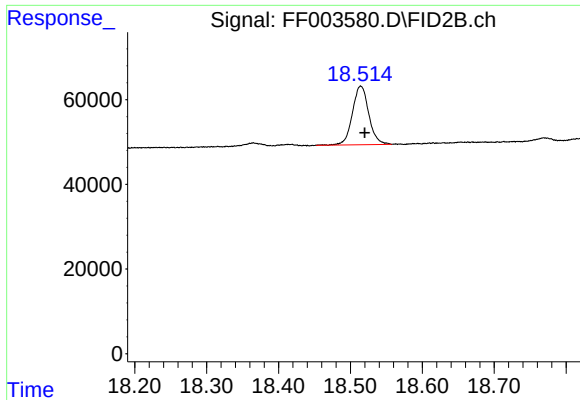


#14 N-DOTRIACONTANE

R.T.: 18.514 min
Delta R.T.: -0.005 min
Response: 218101
Conc: 1.58 ug/ml

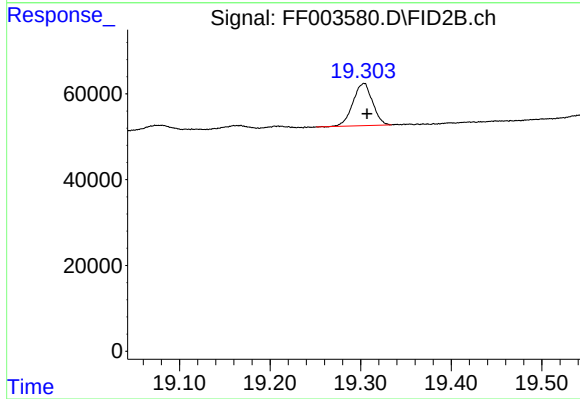

#15 N-TETRATRIACONTANE

R.T.: 19.304 min
Delta R.T.: -0.003 min
Response: 147700
Conc: 1.16 ug/ml

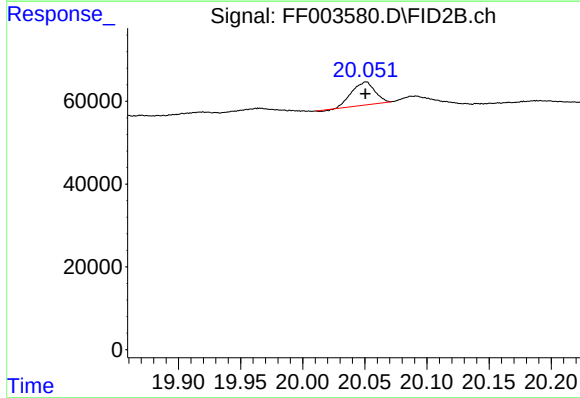

#16 N-HEXATRIACONTANE

R.T.: 20.051 min
Delta R.T.: 0.000 min
Response: 71799
Conc: 0.61 ug/ml