

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022119\
 Data File : FF003596.D
 Signal(s) : FID2B.ch
 Acq On : 21 Feb 2019 21:19
 Operator : AJ\SJ
 Sample : K1344-07 20X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 21 23:56:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.354	123046	0.913 ug/ml
4)	N-TETRADECANE	8.147	258323	1.908 ug/ml
5)	N-HEXADECANE	9.747	304167	2.232 ug/ml
6)	N-OCTADECANE	11.189	223752	1.626 ug/ml
7)	N-EICOSANE	12.501	182865	1.330 ug/ml
8)	N-DOCOSANE	13.704	60643	0.443 ug/ml
10)	N-TETRACOSANE	14.806	301577	2.218 ug/ml
11)	N-HEXACOSANE	15.835	110434	0.814 ug/ml
12)	N-OCTACOSANE	16.789	172833	1.262 ug/ml
13)	N-TRIACONTANE	17.678	256490	1.817 ug/ml
14)	N-DOTRIACONTANE	18.514	294729	2.136 ug/ml
15)	N-TETRATRIACONTANE	19.304	228607	1.802 ug/ml
16)	N-HEXATRIACONTANE	20.049	109701	0.938 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022119\
Data File : FF003596.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2019 21:19
Operator : AJ\SJ
Sample : K1344-07 20X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 23:56:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

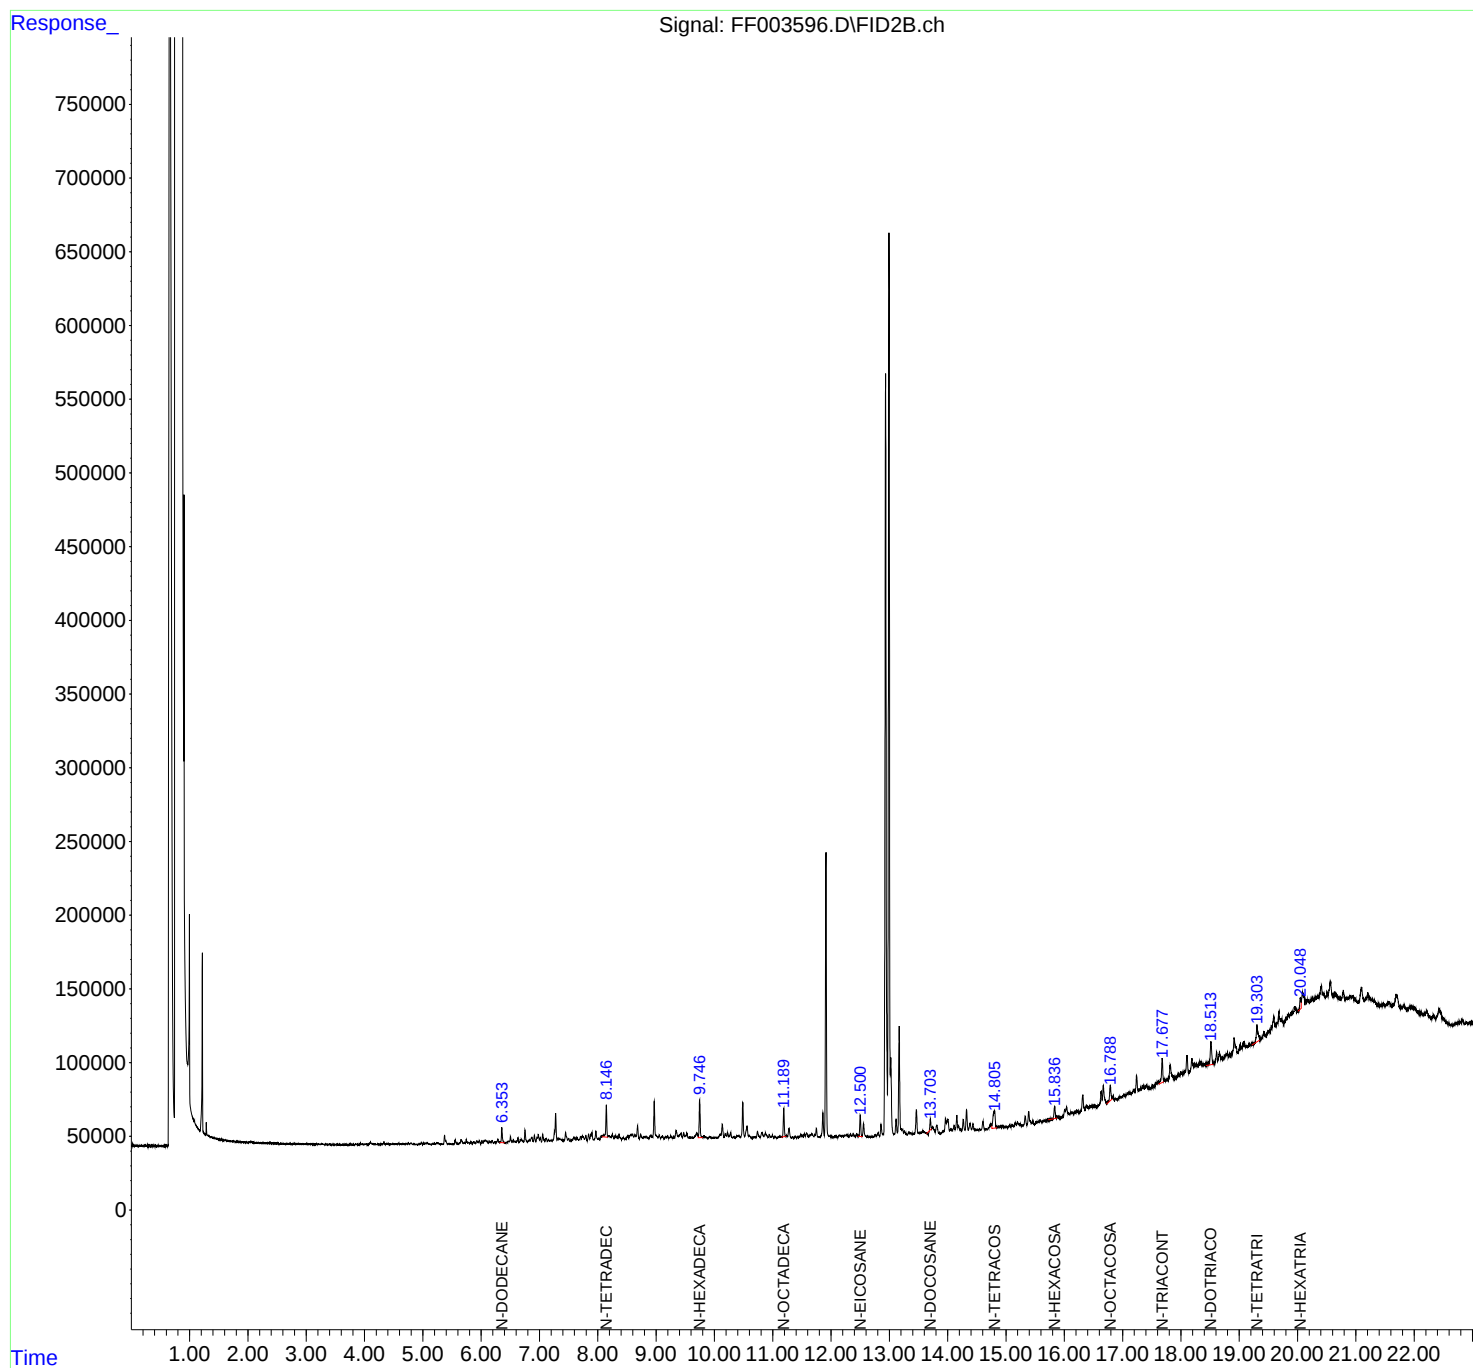

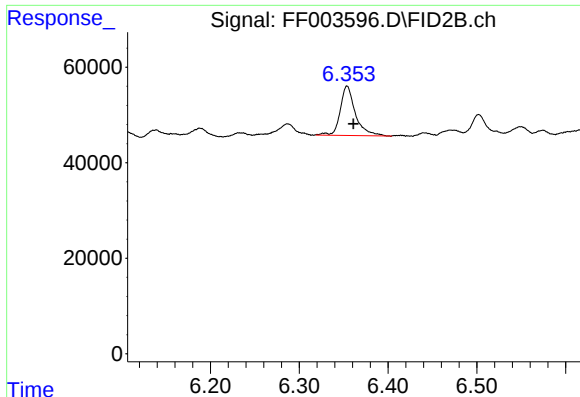


#3 N-DODECANE

R.T.: 6.354 min
Delta R.T.: -0.007 min
Response: 123046
Conc: 0.91 ug/ml

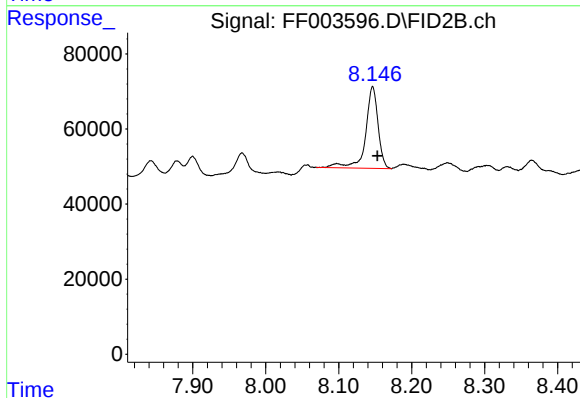


#4 N-TETRADECANE

R.T.: 8.147 min
Delta R.T.: -0.007 min
Response: 258323
Conc: 1.91 ug/ml

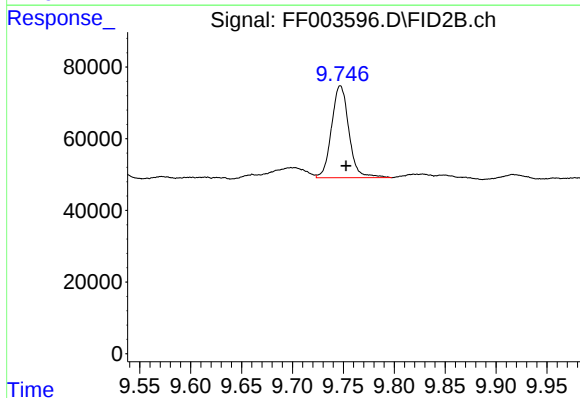


#5 N-HEXADECANE

R.T.: 9.747 min
Delta R.T.: -0.006 min
Response: 304167
Conc: 2.23 ug/ml

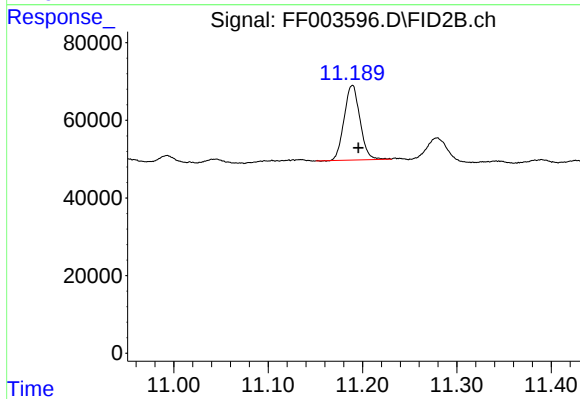


#6 N-OCTADECANE

R.T.: 11.189 min
Delta R.T.: -0.006 min
Response: 223752
Conc: 1.63 ug/ml

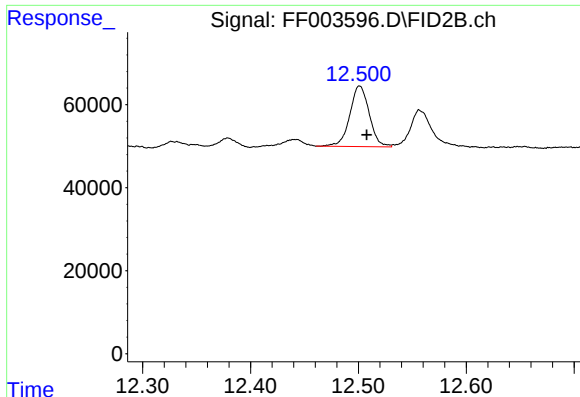


#7 N-EICOSANE

R.T.: 12.501 min
Delta R.T.: -0.007 min
Response: 182865
Conc: 1.33 ug/ml

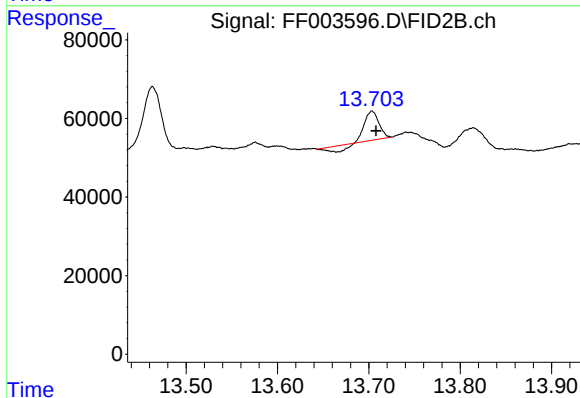


#8 N-DOCOSANE

R.T.: 13.704 min
Delta R.T.: -0.004 min
Response: 60643
Conc: 0.44 ug/ml

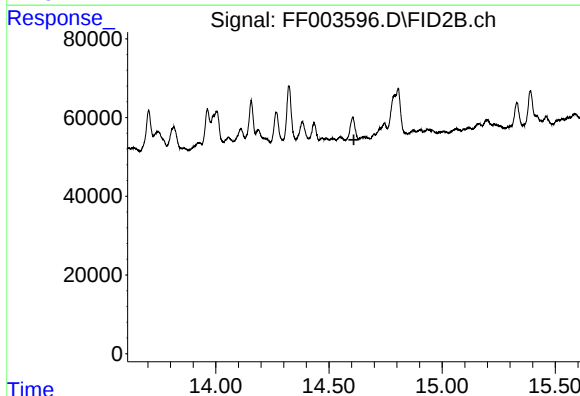


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.610 min
Response: 0
Conc: N.D.

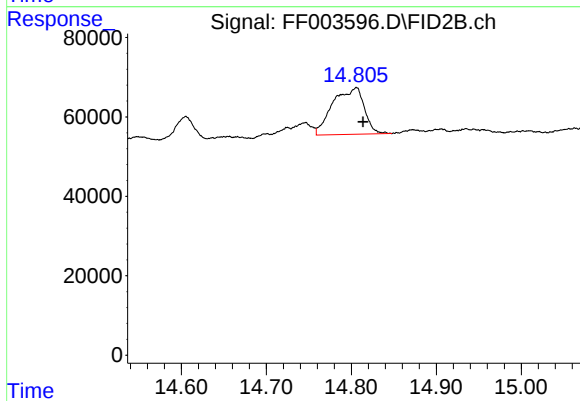


#10 N-TETRACOSANE

R.T.: 14.806 min
Delta R.T.: -0.008 min
Response: 301577
Conc: 2.22 ug/ml

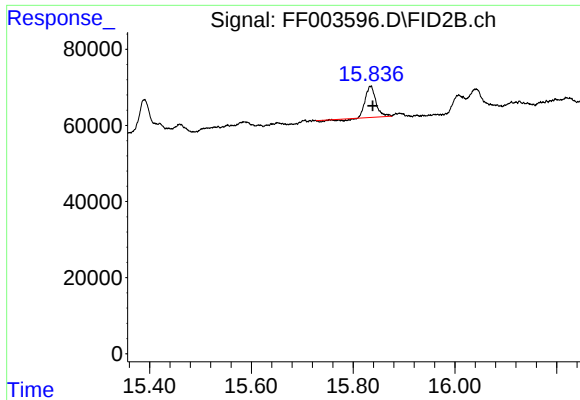


#11 N-HEXACOSANE

R.T.: 15.835 min
Delta R.T.: -0.004 min
Response: 110434
Conc: 0.81 ug/ml

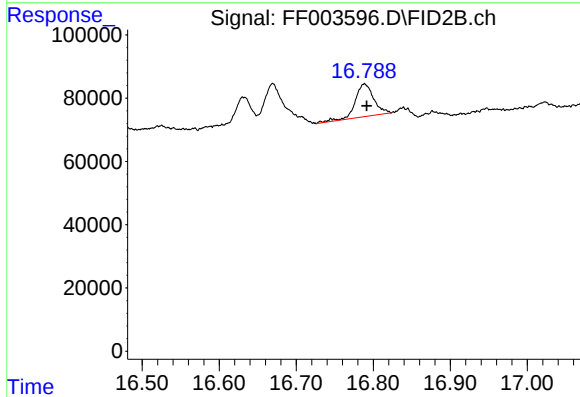


#12 N-OCTACOSANE

R.T.: 16.789 min
Delta R.T.: -0.003 min
Response: 172833
Conc: 1.26 ug/ml

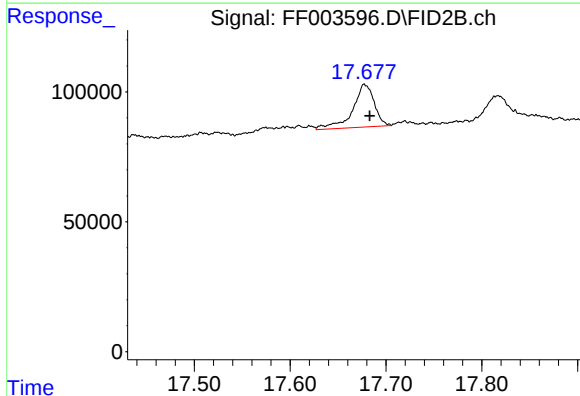


#13 N-TRIACONTANE

R.T.: 17.678 min
Delta R.T.: -0.005 min
Response: 256490
Conc: 1.82 ug/ml

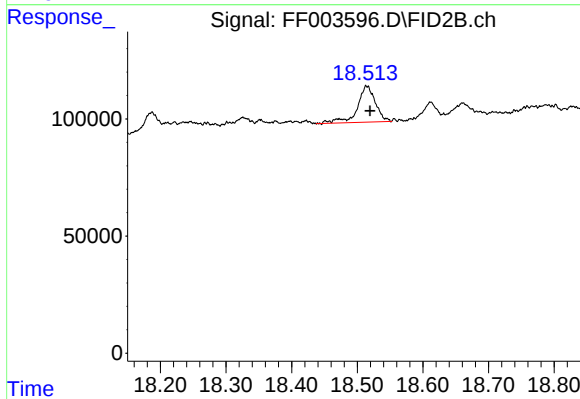


#14 N-DOTRIACONTANE

R.T.: 18.514 min
Delta R.T.: -0.005 min
Response: 294729
Conc: 2.14 ug/ml

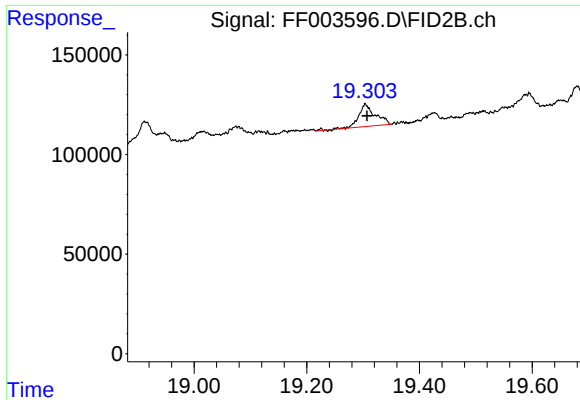

#15 N-TETRATRIACONTANE

R.T.: 19.304 min
Delta R.T.: -0.003 min
Response: 228607
Conc: 1.80 ug/ml

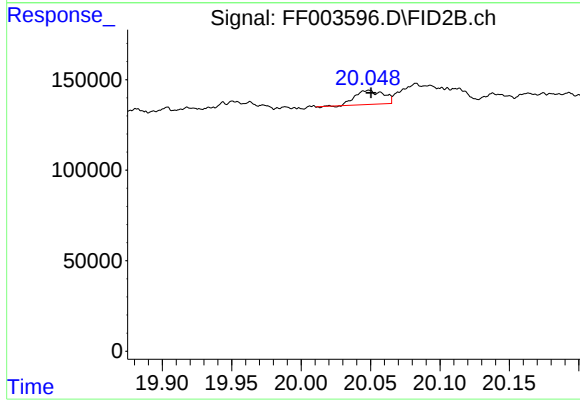

#16 N-HEXATRIACONTANE

R.T.: 20.049 min
Delta R.T.: -0.002 min
Response: 109701
Conc: 0.94 ug/ml