

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
 Data File : FF006437.D
 Signal(s) : FID2B.ch
 Acq On : 21 Feb 2020 11:28
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 21 22:54:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
3) N-DODECANE	6.383	3028253	22.157	ug/ml
10) N-TETRACOSANE	14.785	147368	1.055	ug/ml
12) N-OCTACOSANE	16.770	3084895	22.353	ug/ml
13) N-TRIACONTANE	17.651	204483	1.479	ug/ml
14) N-DOTRIACONTANE	18.481	209800	1.595	ug/ml
15) N-TETRATRIACONTANE	19.260	147797	1.316	ug/ml
16) N-HEXATRIACONTANE	19.999	100454	1.038	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
Data File : FF006437.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2020 11:28
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 22:54:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

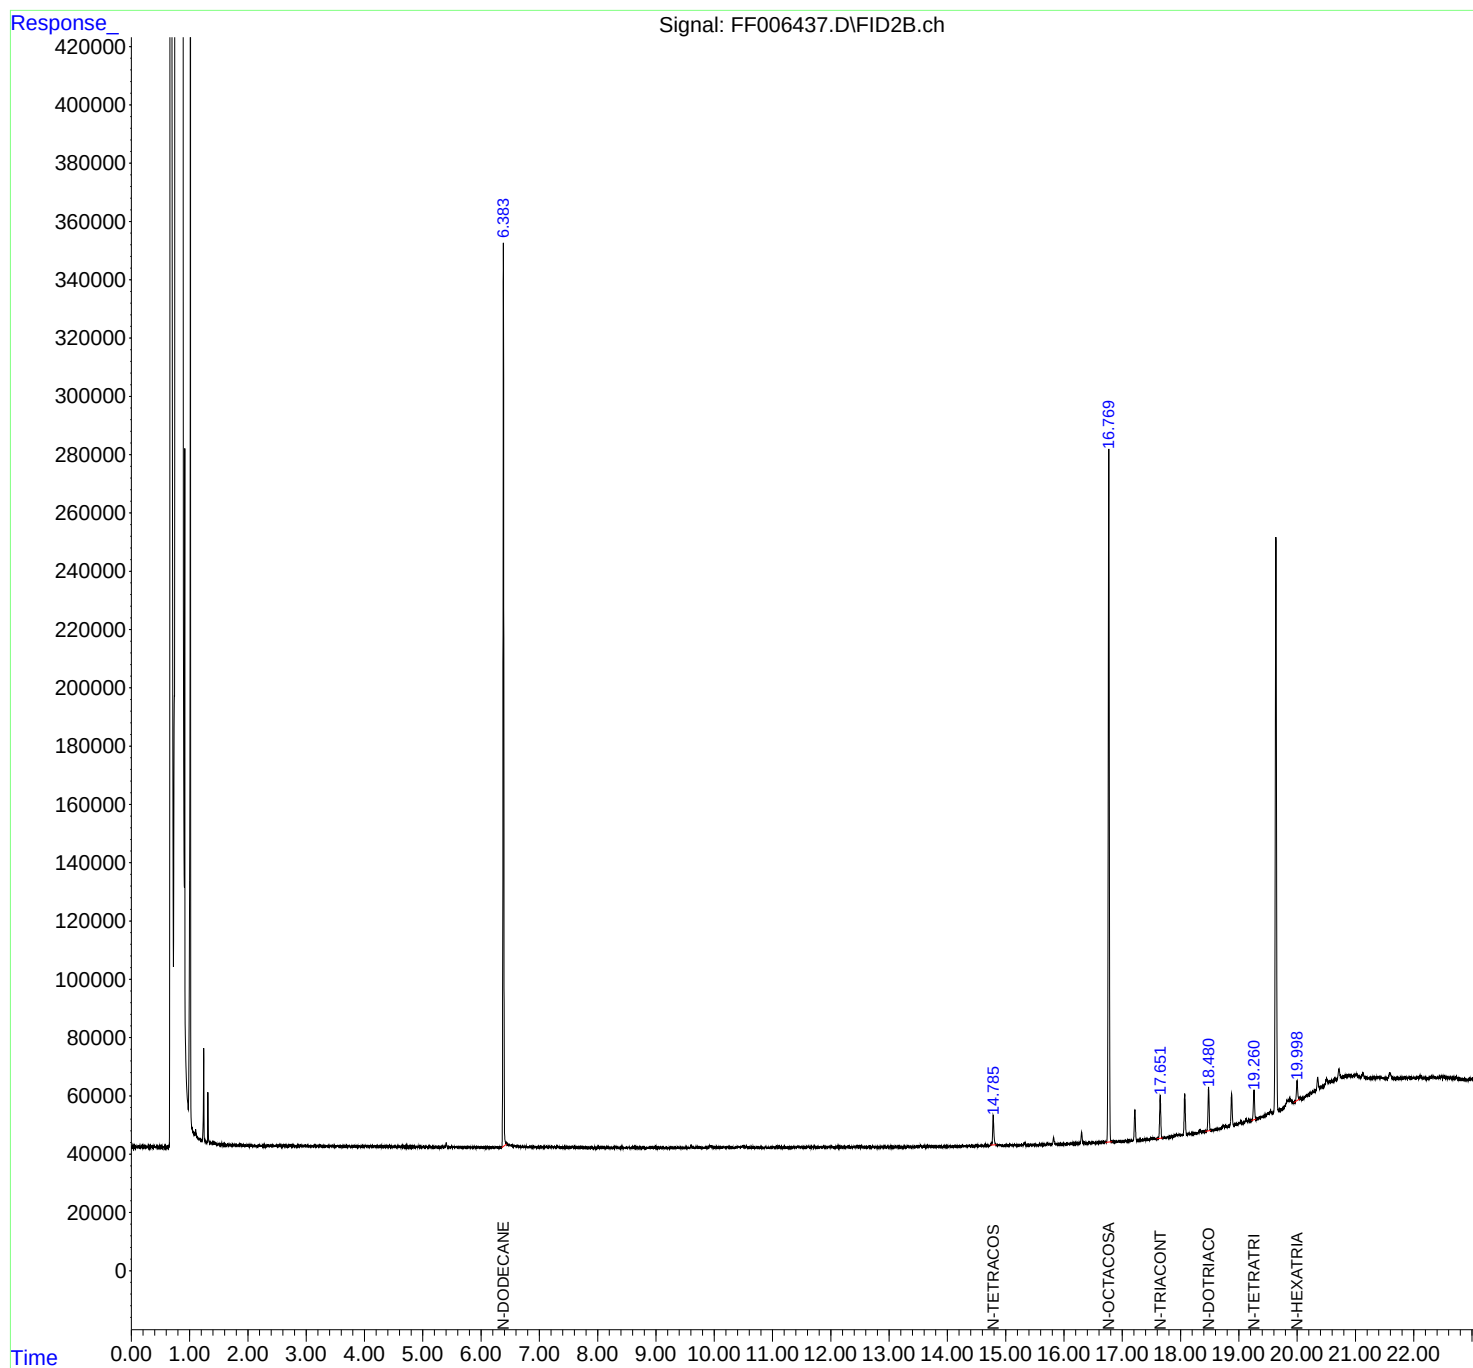


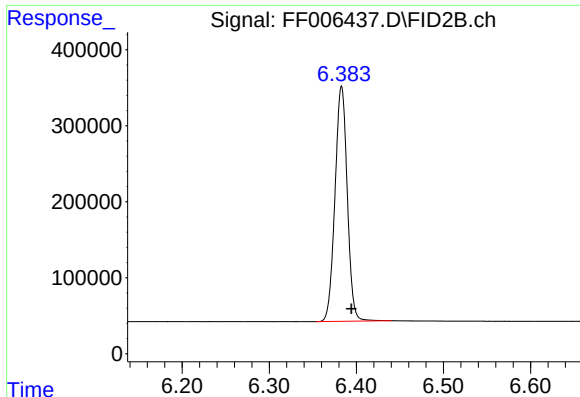

#3 N-DODECANE


R.T.: 6.383 min
Delta R.T.: -0.011 min
Response: 3028253
Conc: 22.16 ug/ml

Instrument :
FID_F
ClientSampleId :

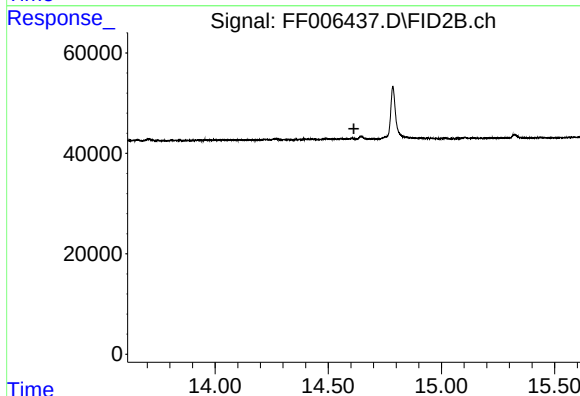


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.613 min
Response: 0
Conc: N.D.

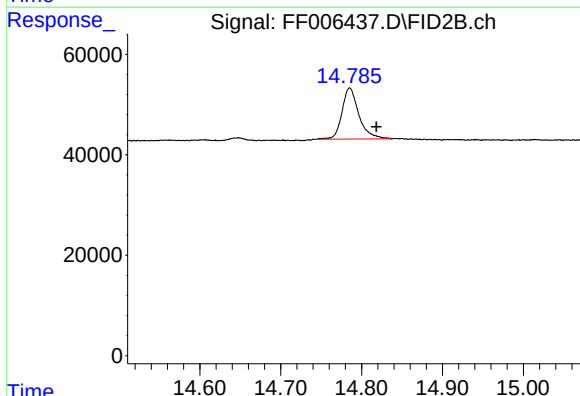


#10 N-TETRACOSANE

R.T.: 14.785 min
Delta R.T.: -0.033 min
Response: 147368
Conc: 1.05 ug/ml

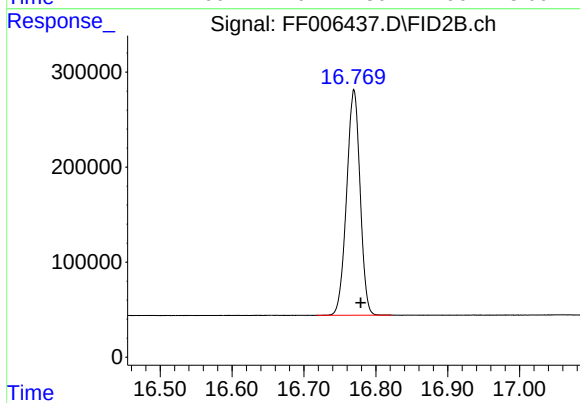

#12 N-OCTACOSANE


R.T.: 16.770 min
Delta R.T.: -0.009 min
Response: 3084895
Conc: 22.35 ug/ml

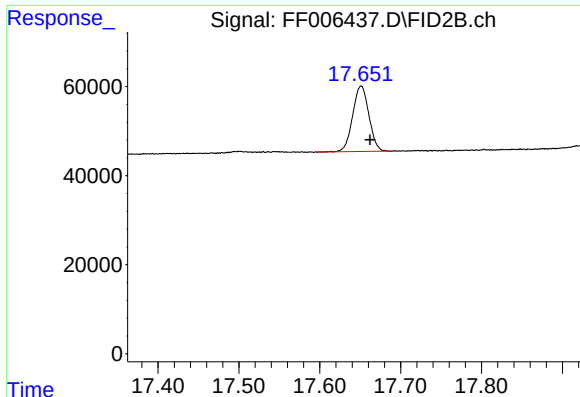

#13 N-TRIACONTANE


R.T.: 17.651 min
Delta R.T.: -0.011 min
Response: 204483
Conc: 1.48 ug/ml

Instrument :
FID_F
ClientSampleId :

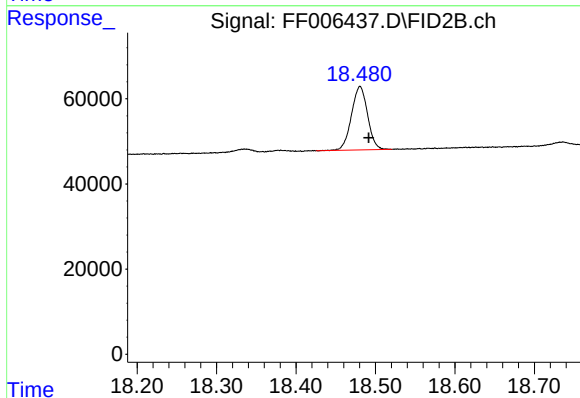


#14 N-DOTRIACONTANE

R.T.: 18.481 min
Delta R.T.: -0.011 min
Response: 209800
Conc: 1.59 ug/ml

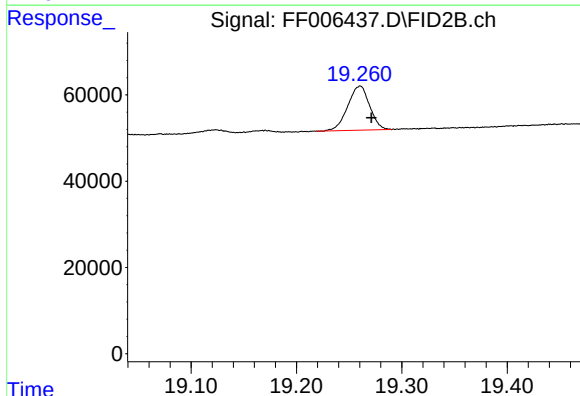

#15 N-TETRATRIACONTANE

R.T.: 19.260 min
Delta R.T.: -0.011 min
Response: 147797
Conc: 1.32 ug/ml

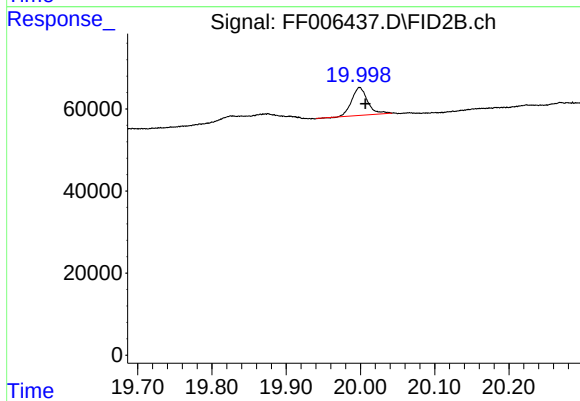

#16 N-HEXATRIACONTANE

R.T.: 19.999 min
Delta R.T.: -0.008 min
Response: 100454
Conc: 1.04 ug/ml