

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
 Data File : FF006438.D
 Signal(s) : FID2B.ch
 Acq On : 21 Feb 2020 13:37
 Operator : DD\AJ
 Sample : L1576-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 21 22:55:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.602	1482240	12.167 ug/ml
Target Compounds			
4) N-TETRADECANE	8.226	182554	1.327 ug/ml
7) N-EICOSANE	12.571	177425	1.259 ug/ml
10) N-TETRACOSANE	14.850	83595	0.598 ug/ml
11) N-HEXACOSANE	15.823	420850	3.049 ug/ml
12) N-OCTACOSANE	16.770	1226864	8.890 ug/ml
13) N-TRIACONTANE	17.657	1670481	12.079 ug/ml
14) N-DOTRIACONTANE	18.484	1985231	15.090 ug/ml
15) N-TETRATRIACONTANE	19.268	730131	6.501 ug/ml
16) N-HEXATRIACONTANE	20.006	784008	8.101 ug/ml
17) N-OCTATRIACONTANE	20.718	34892	0.494 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
Data File : FF006438.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2020 13:37
Operator : DD\AJ
Sample : L1576-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 22:55:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

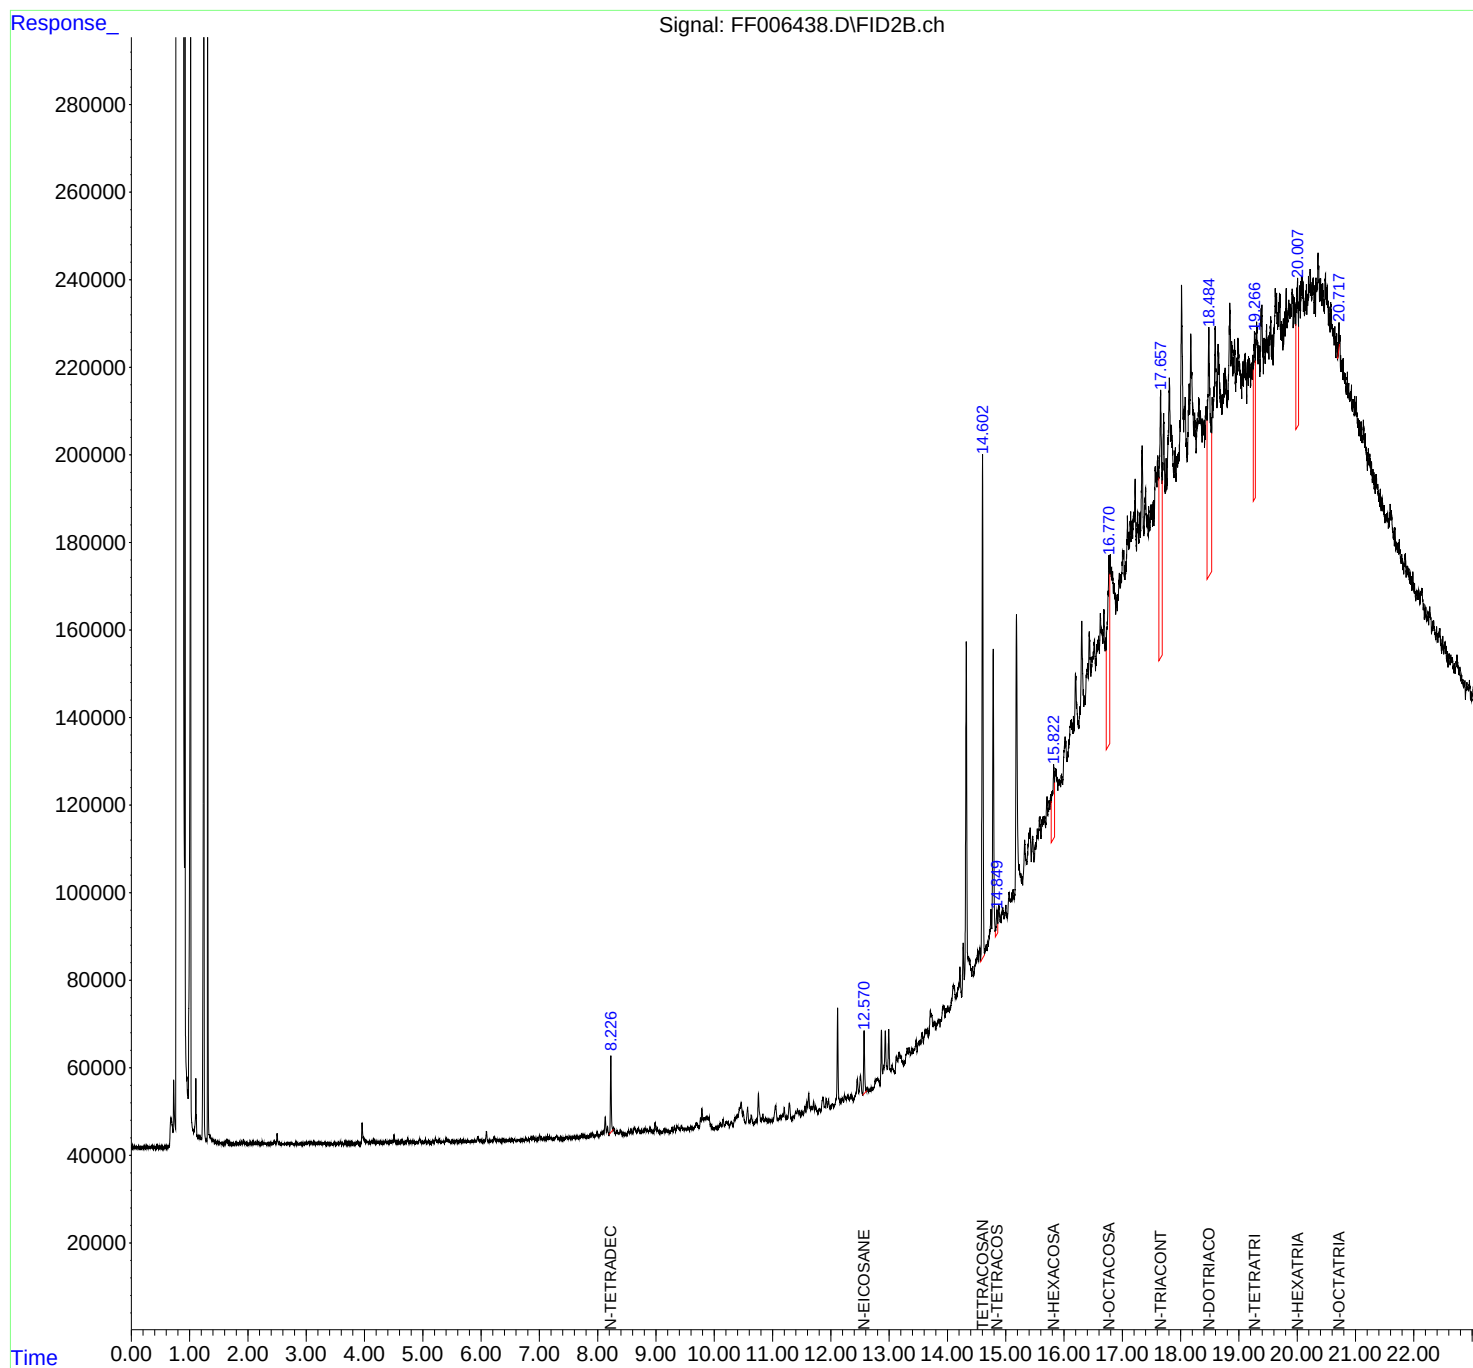


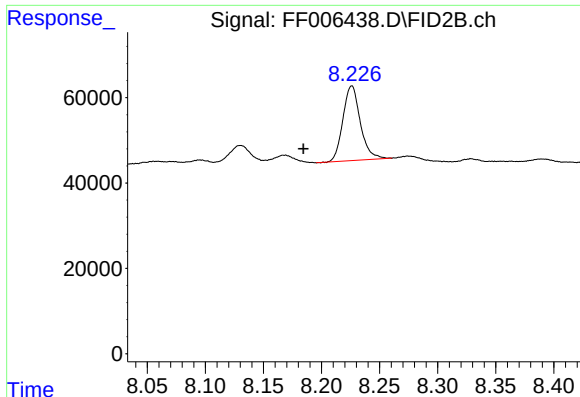

#4 N-TETRADECANE


R.T.: 8.226 min
Delta R.T.: 0.042 min
Response: 182554
Conc: 1.33 ug/ml

Instrument :
FID_F
ClientSampleId :

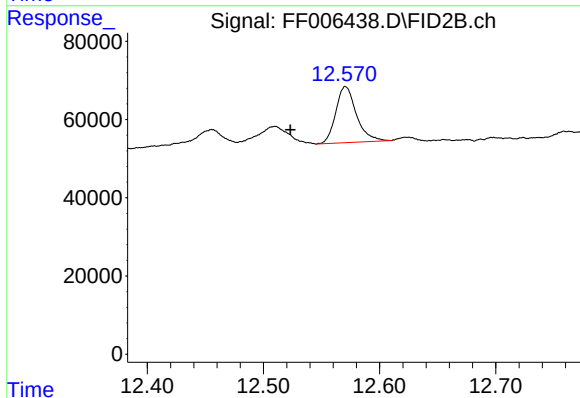


#7 N-EICOSANE

R.T.: 12.571 min
Delta R.T.: 0.048 min
Response: 177425
Conc: 1.26 ug/ml

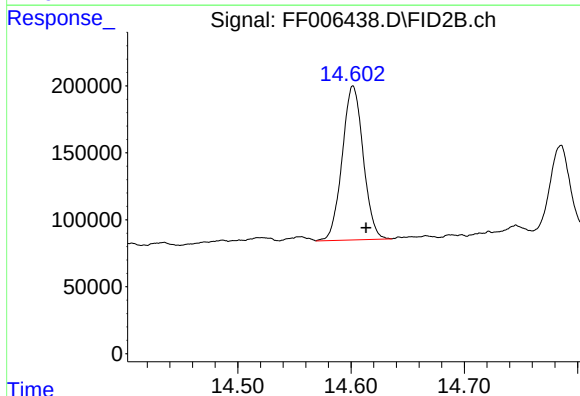


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.602 min
Delta R.T.: -0.011 min
Response: 1482240
Conc: 12.17 ug/ml

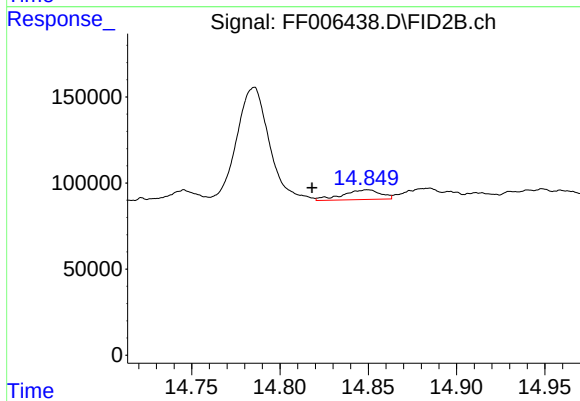

#10 N-TETRACOSANE


R.T.: 14.850 min
Delta R.T.: 0.032 min
Response: 83595
Conc: 0.60 ug/ml

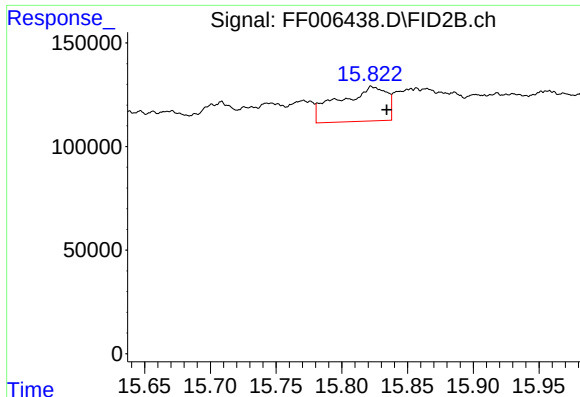

#11 N-HEXACOSANE


R.T.: 15.823 min
Delta R.T.: -0.011 min
Response: 420850
Conc: 3.05 ug/ml

Instrument :
FID_F
ClientSampleId :

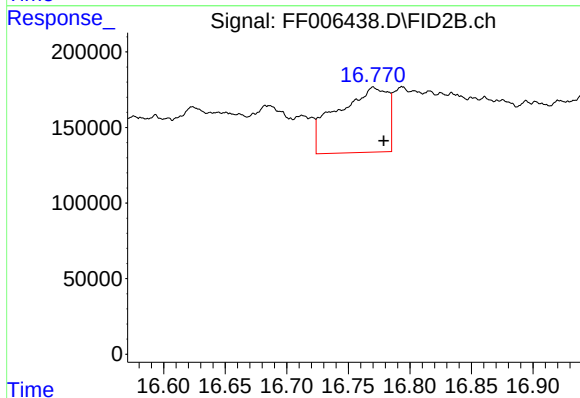


#12 N-OCTACOSANE

R.T.: 16.770 min
Delta R.T.: -0.009 min
Response: 1226864
Conc: 8.89 ug/ml

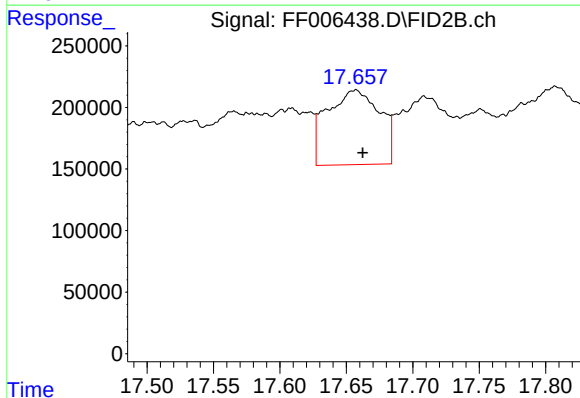


#13 N-TRIACONTANE

R.T.: 17.657 min
Delta R.T.: -0.005 min
Response: 1670481
Conc: 12.08 ug/ml

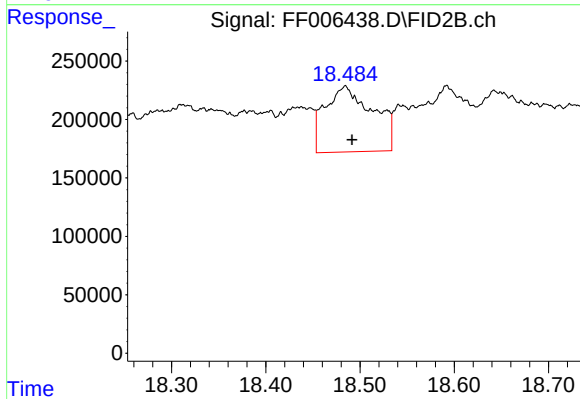

#14 N-DOTRIACONTANE

R.T.: 18.484 min
Delta R.T.: -0.007 min
Response: 1985231
Conc: 15.09 ug/ml

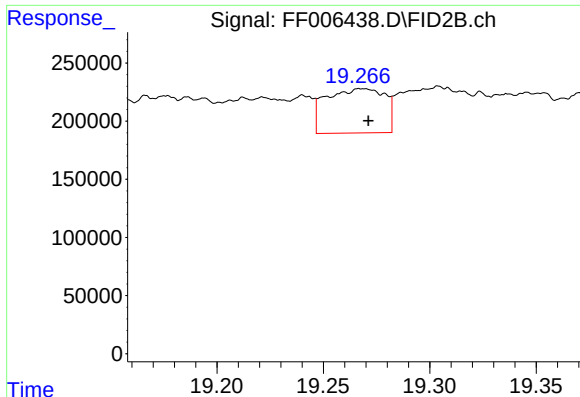

#15 N-TETRATRIACONTANE


R.T.: 19.268 min

Delta R.T.: -0.003 min

Response: 730131

Conc: 6.50 ug/ml

Instrument :
FID_F
ClientSampleId :

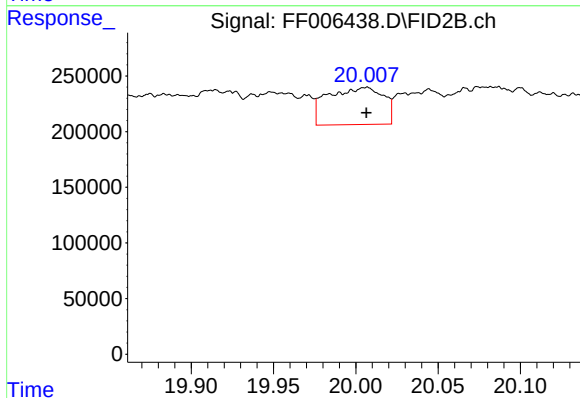


#16 N-HEXATRIACONTANE

R.T.: 20.006 min

Delta R.T.: 0.000 min

Response: 784008

Conc: 8.10 ug/ml

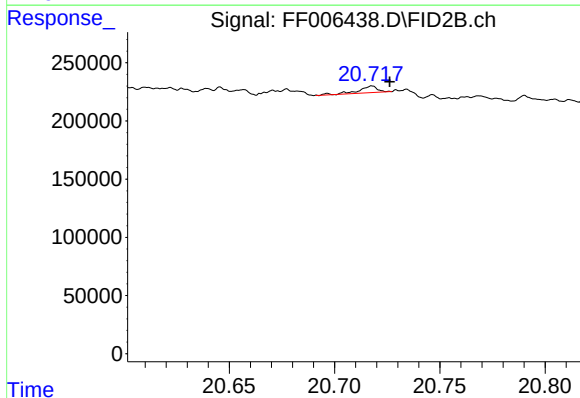

#17 N-OCTATRIACONTANE

R.T.: 20.718 min

Delta R.T.: -0.009 min

Response: 34892

Conc: 0.49 ug/ml