

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
 Data File : FF006446.D
 Signal(s) : FID2B.ch
 Acq On : 21 Feb 2020 17:37
 Operator : DD\AJ
 Sample : L1605-01
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 21 22:55:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.608	2091923	17.171 ug/ml
Target Compounds			
4) N-TETRADECANE	8.237f	101581	0.739 ug/ml
7) N-EICOSANE	12.580f	122636	0.870 ug/ml
10) N-TETRACOSANE	14.792	202419	1.449 ug/ml
11) N-HEXACOSANE	15.826	111364	0.807 ug/ml
12) N-OCTACOSANE	16.773	320447	2.322 ug/ml
13) N-TRIACONTANE	17.657	390017	2.820 ug/ml
14) N-DOTRIACONTANE	18.483	375584	2.855 ug/ml
16) N-HEXATRIACONTANE	19.985	285058	2.945 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
Data File : FF006446.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2020 17:37
Operator : DD\AJ
Sample : L1605-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 22:55:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

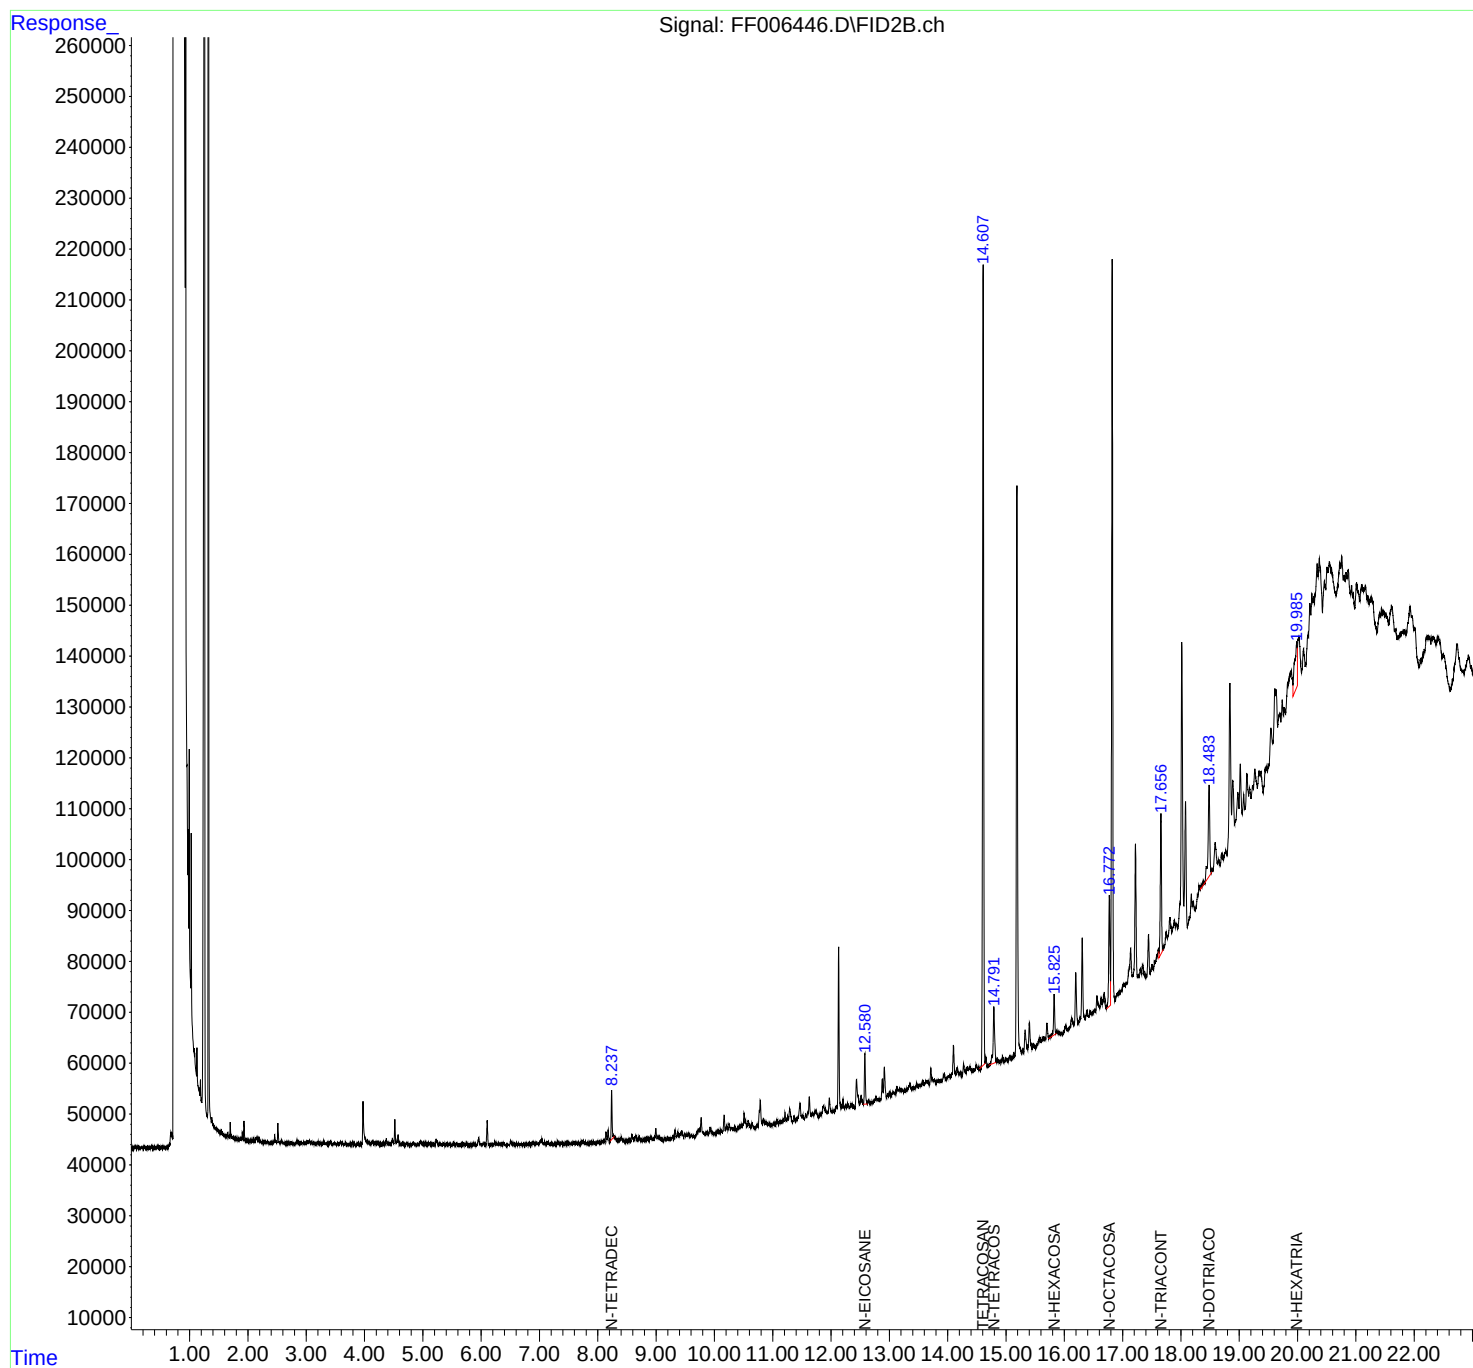


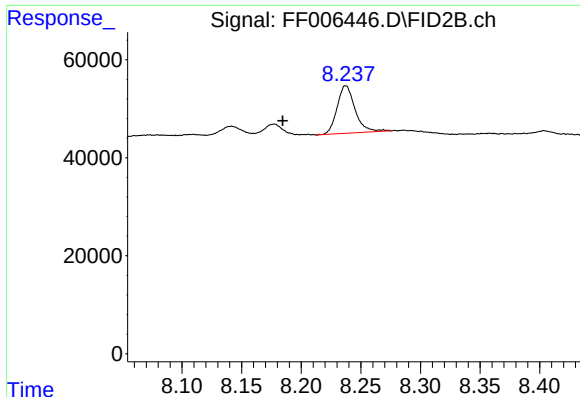

#4 N-TETRADECANE


R.T.: 8.237 min
Delta R.T.: 0.053 min
Response: 101581
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

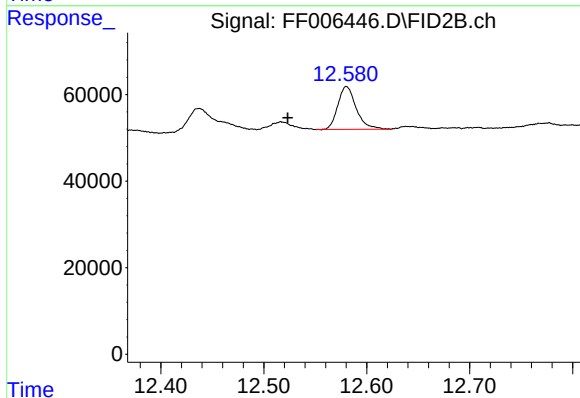


#7 N-EICOSANE

R.T.: 12.580 min
Delta R.T.: 0.057 min
Response: 122636
Conc: 0.87 ug/ml

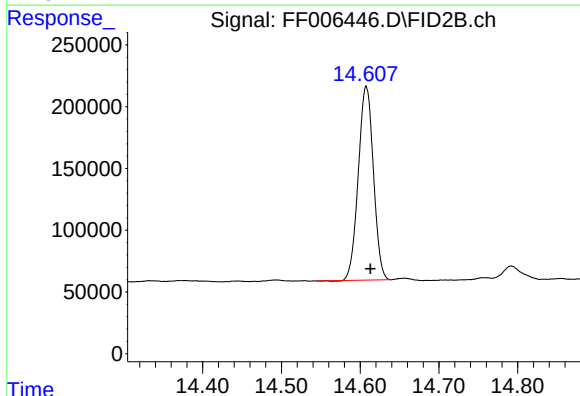


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.608 min
Delta R.T.: -0.005 min
Response: 2091923
Conc: 17.17 ug/ml

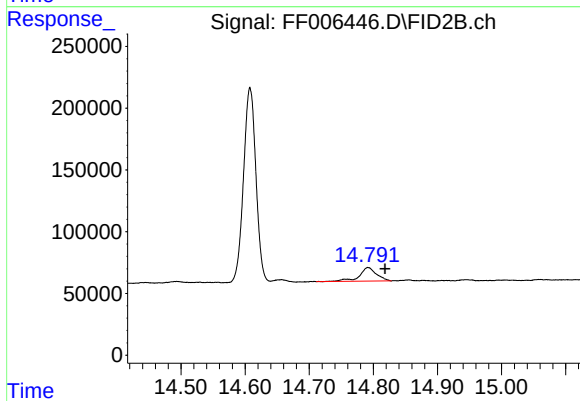

#10 N-TETRACOSANE


R.T.: 14.792 min
Delta R.T.: -0.026 min
Response: 202419
Conc: 1.45 ug/ml

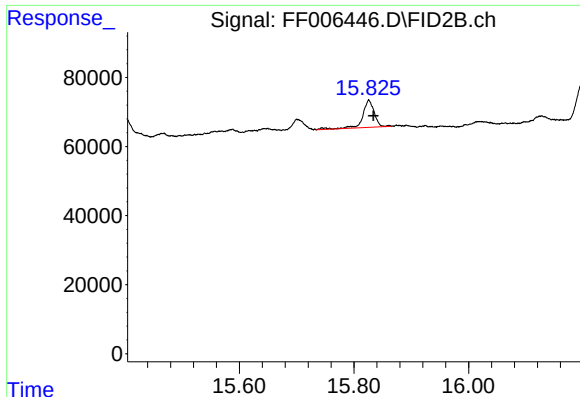

#11 N-HEXACOSANE


R.T.: 15.826 min
Delta R.T.: -0.008 min
Response: 111364
Conc: 0.81 ug/ml

Instrument :
FID_F
ClientSampleId :

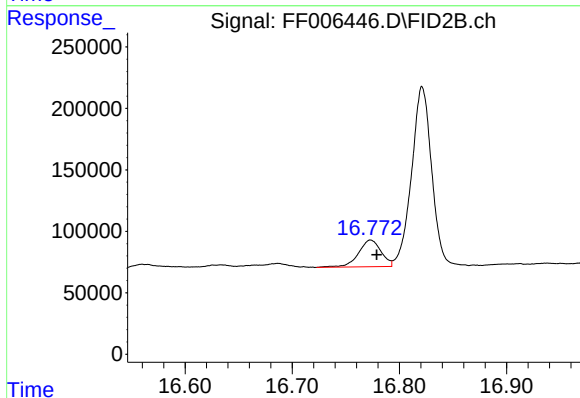


#12 N-OCTACOSANE

R.T.: 16.773 min
Delta R.T.: -0.006 min
Response: 320447
Conc: 2.32 ug/ml

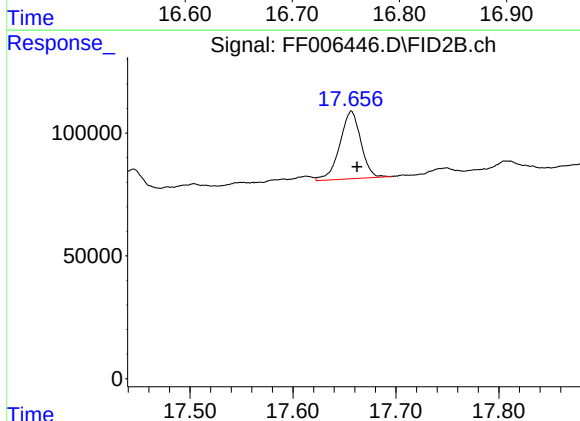


#13 N-TRIACONTANE

R.T.: 17.657 min
Delta R.T.: -0.006 min
Response: 390017
Conc: 2.82 ug/ml

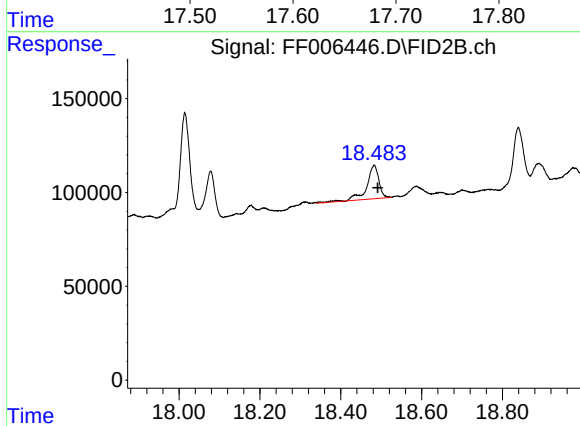

#14 N-DOTRIACONTANE

R.T.: 18.483 min
Delta R.T.: -0.008 min
Response: 375584
Conc: 2.85 ug/ml

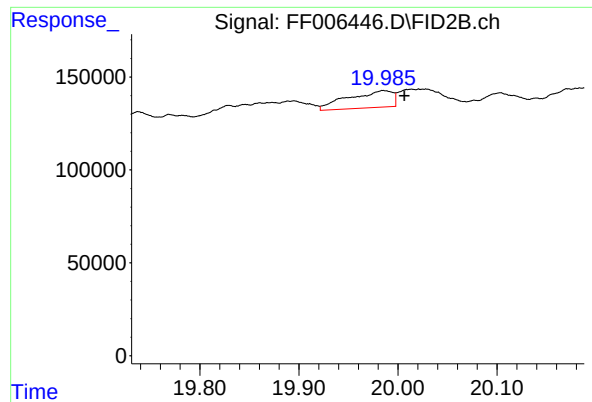

#16 N-HEXATRIACONTANE

R.T.: 19.985 min
Delta R.T.: -0.021 min
Response: 285058
Conc: 2.95 ug/ml

Instrument :
FID_F
ClientSampleId :