

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
 Data File : FF006447.D
 Signal(s) : FID2B.ch
 Acq On : 21 Feb 2020 18:07
 Operator : DD\AJ
 Sample : PB126998BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 21 22:56:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.607	1852691	15.207 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.790	117557	0.841 ug/ml
14)	N-DOTRIACONTANE	18.484	35312	0.268 ug/ml
15)	N-TETRATRIACONTANE	19.264	309954	2.760 ug/ml
16)	N-HEXATRIACONTANE	20.002	1398658	14.452 ug/ml
17)	N-OCTATRIACONTANE	20.711	264542	3.746 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
Data File : FF006447.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2020 18:07
Operator : DD\AJ
Sample : PB126998BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 22:56:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

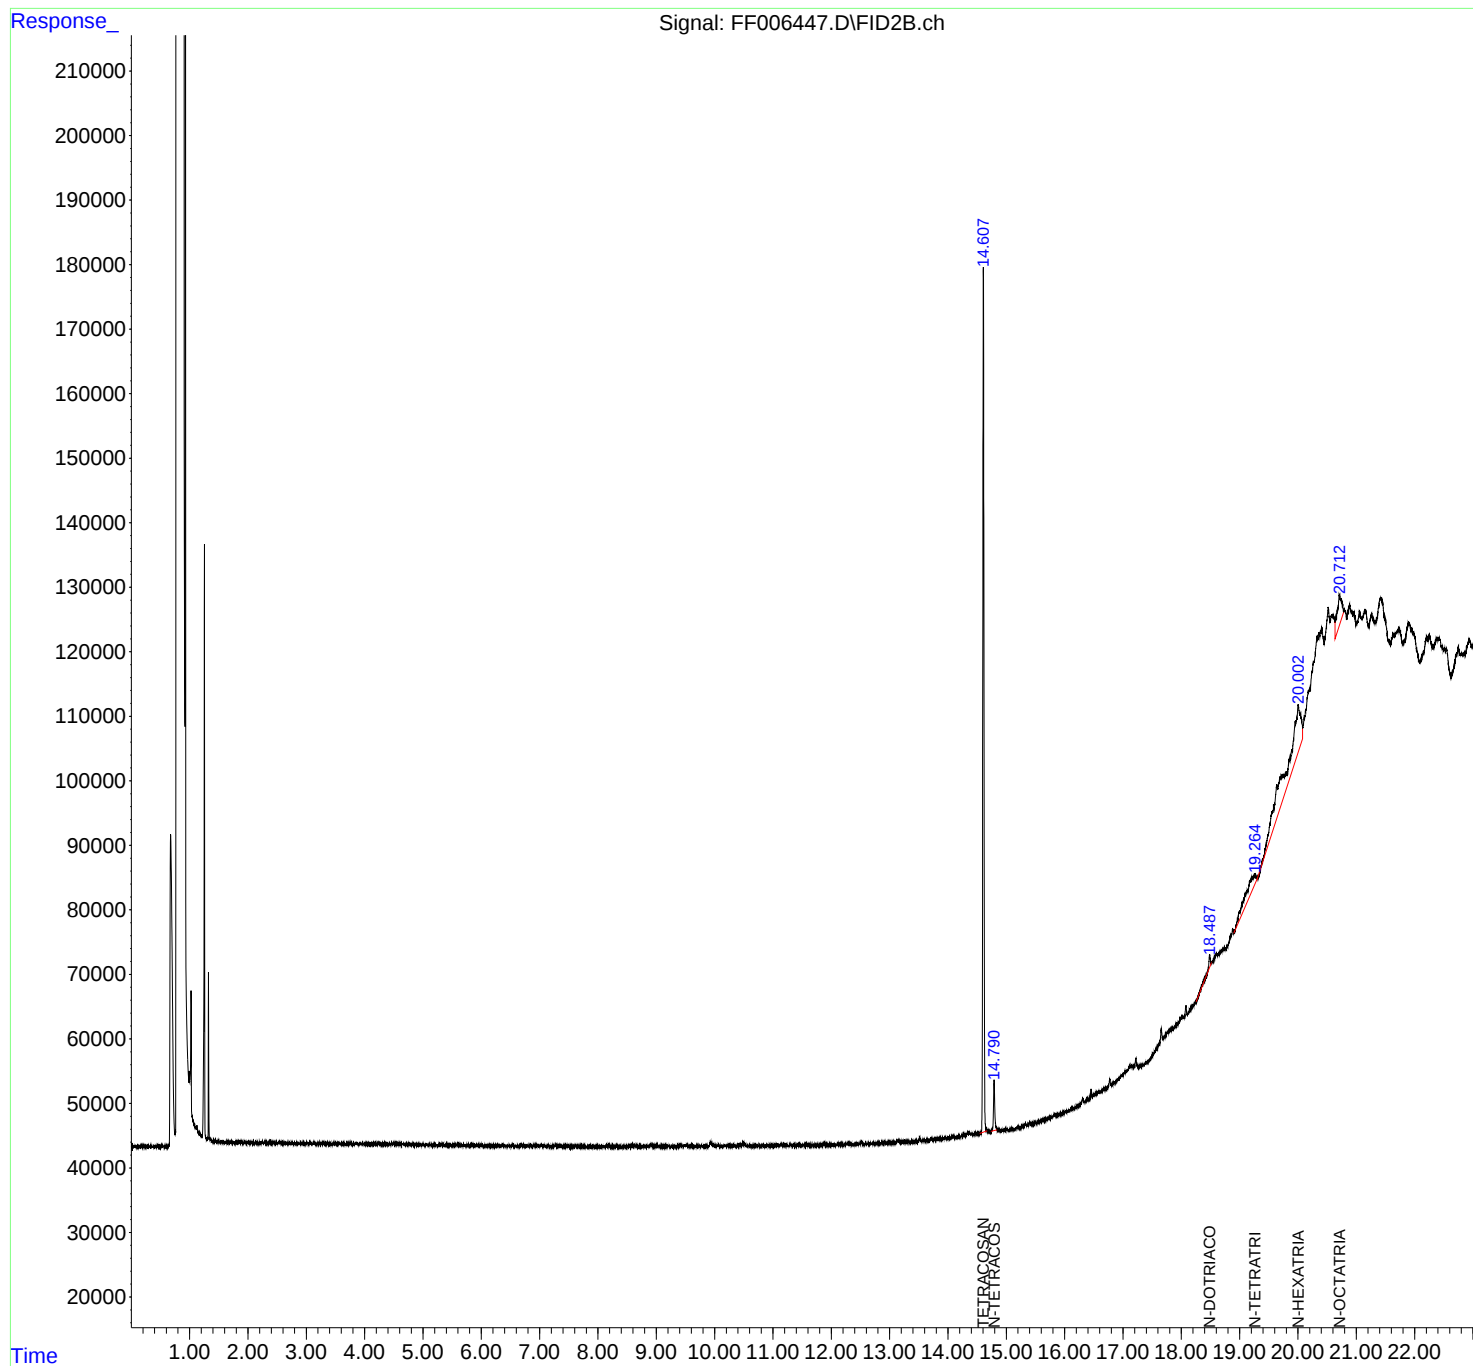


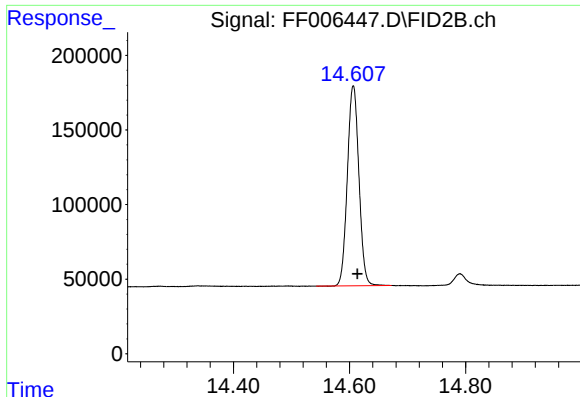

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.607 min
Delta R.T.: -0.007 min
Response: 1852691
Conc: 15.21 ug/ml

Instrument :
FID_F
ClientSampleId :

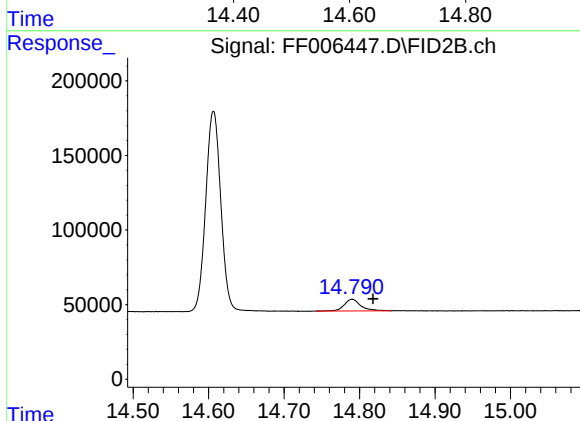


#10 N-TETRACOSANE

R.T.: 14.790 min
Delta R.T.: -0.028 min
Response: 117557
Conc: 0.84 ug/ml

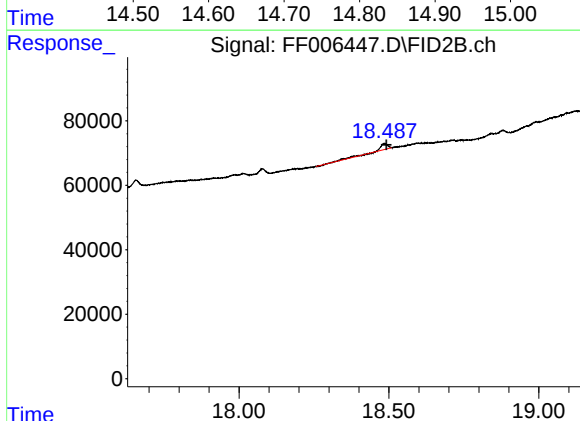


#14 N-DOTRIACONTANE

R.T.: 18.484 min
Delta R.T.: -0.007 min
Response: 35312
Conc: 0.27 ug/ml

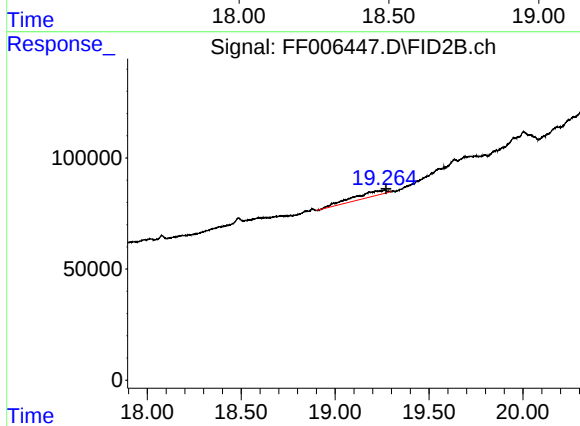

#15 N-TETRATRIACONTANE


R.T.: 19.264 min
Delta R.T.: -0.007 min
Response: 309954
Conc: 2.76 ug/ml

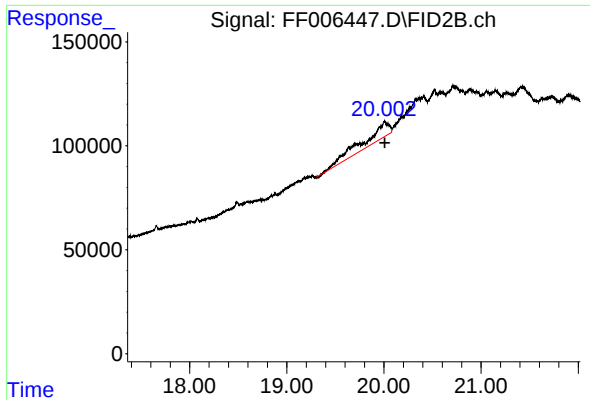

#16 N-HEXATRIACONTANE

R.T.: 20.002 min
Delta R.T.: -0.004 min
Response: 1398658
Conc: 14.45 ug/ml

Instrument :
FID_F
ClientSampleId :

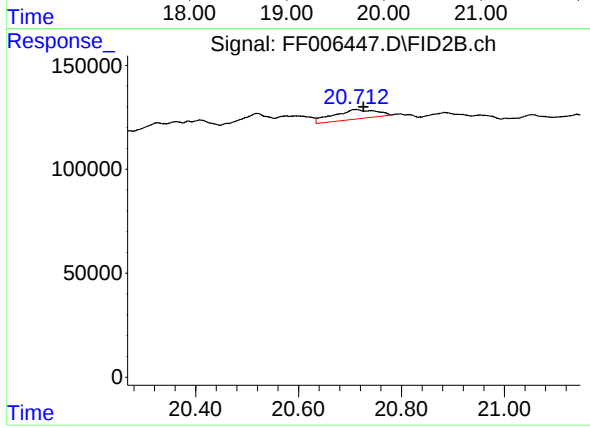

#17 N-OCTATRIACONTANE

R.T.: 20.711 min
Delta R.T.: -0.016 min
Response: 264542
Conc: 3.75 ug/ml