

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
 Data File : FF006450.D
 Signal(s) : FID2B.ch
 Acq On : 21 Feb 2020 19:38
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 21 22:56:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.607	2175122	17.854 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.790	107512	0.769 ug/ml
13) N-TRIACONTANE	17.654	122786	0.888 ug/ml
14) N-DOTRIACONTANE	18.483	135937	1.033 ug/ml
15) N-TETRATRIACONTANE	19.264	92589	0.824 ug/ml
16) N-HEXATRIACONTANE	20.002	121563	1.256 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
Data File : FF006450.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2020 19:38
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 22:56:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

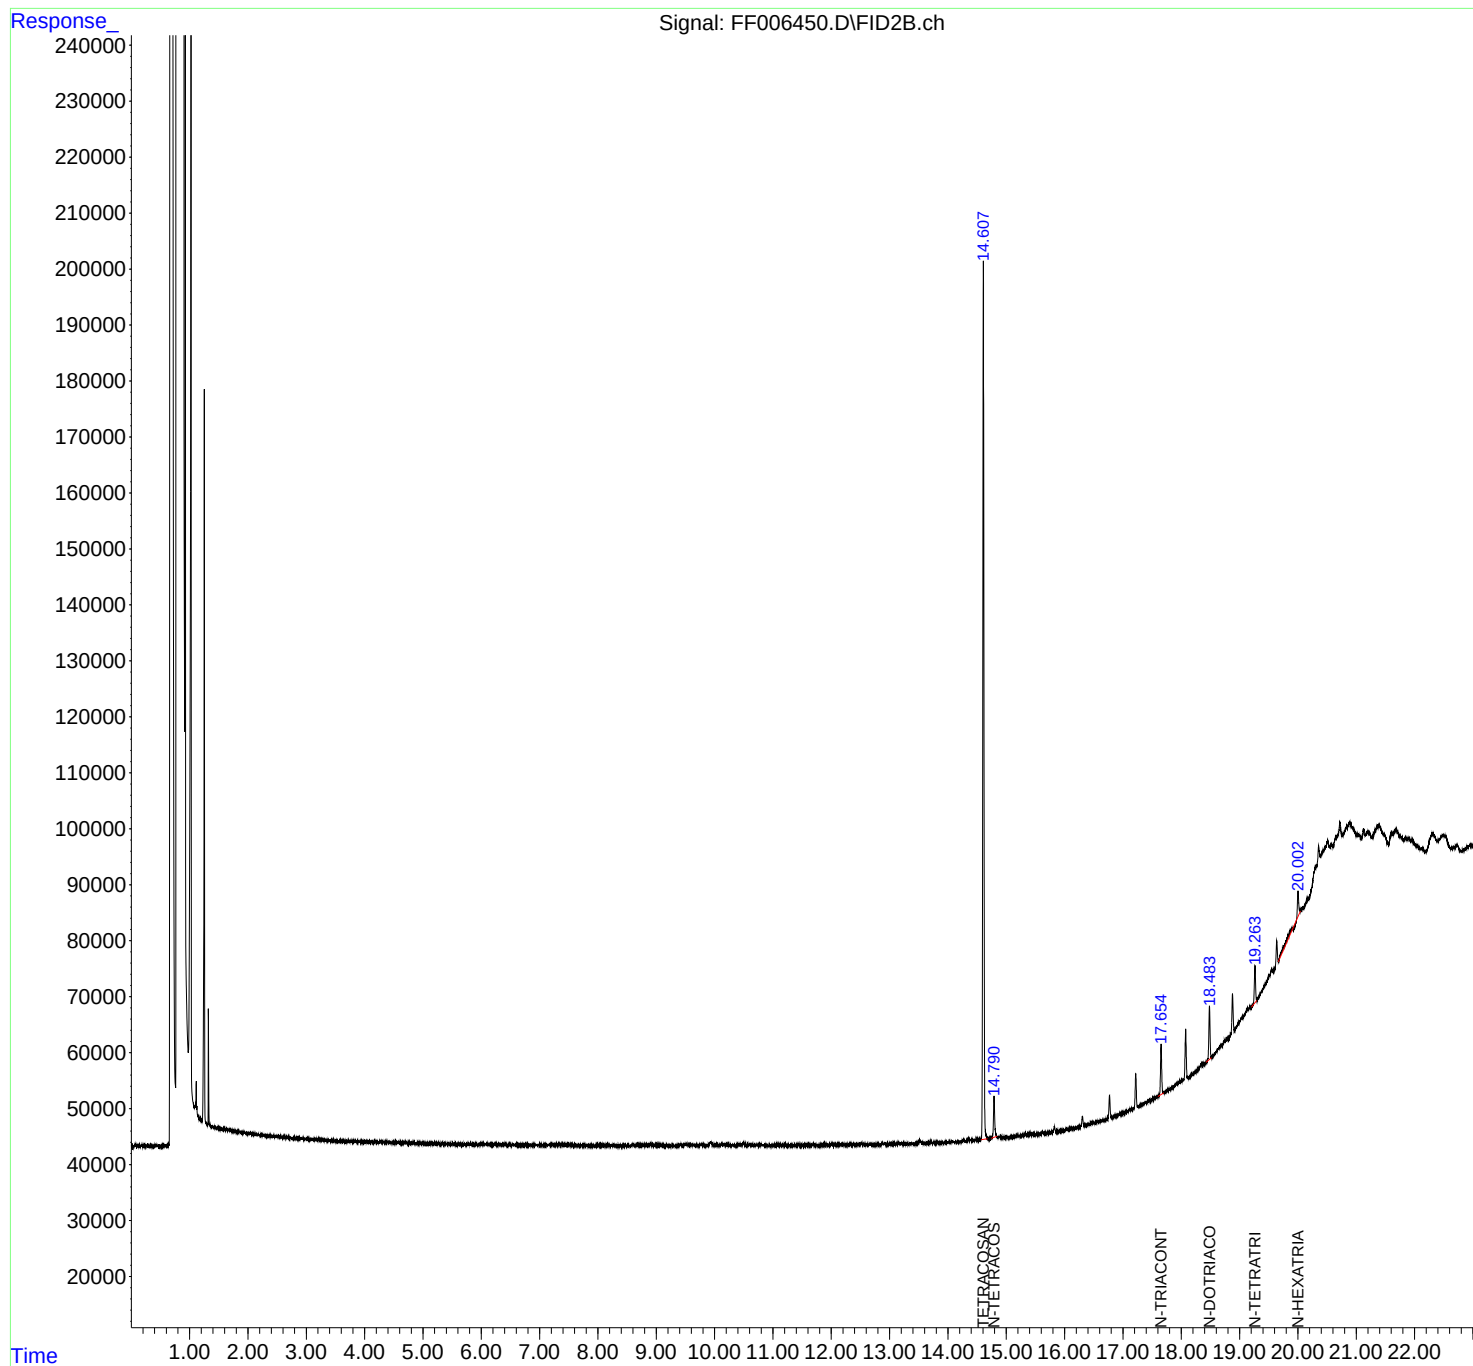


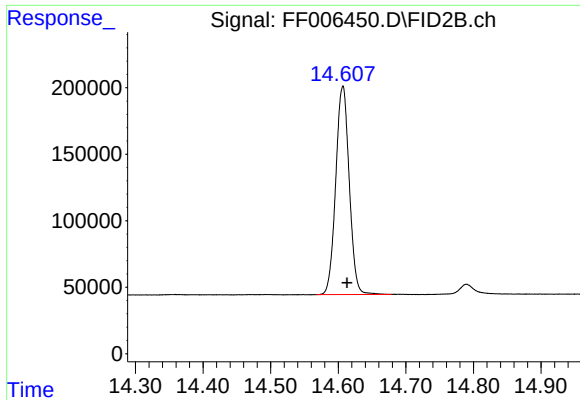

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.607 min
Delta R.T.: -0.006 min
Response: 2175122
Conc: 17.85 ug/ml

Instrument :
FID_F
ClientSampleId :

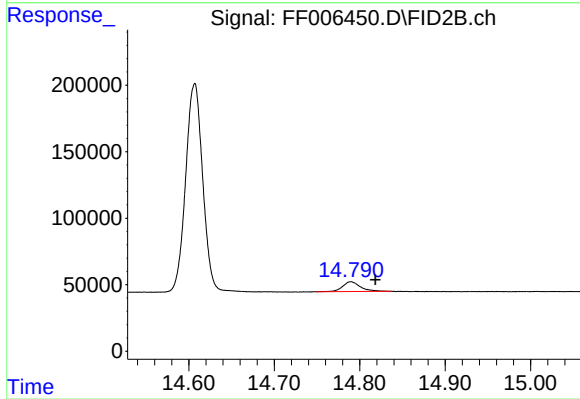


#10 N-TETRACOSANE

R.T.: 14.790 min
Delta R.T.: -0.028 min
Response: 107512
Conc: 0.77 ug/ml

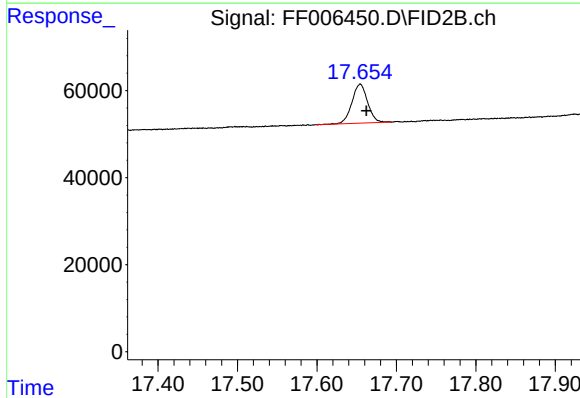


#13 N-TRIACONTANE

R.T.: 17.654 min
Delta R.T.: -0.008 min
Response: 122786
Conc: 0.89 ug/ml

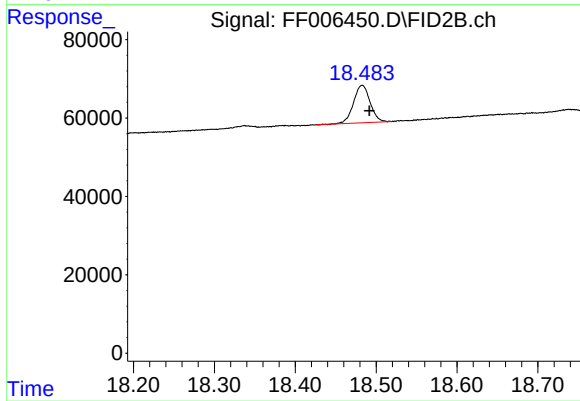

#14 N-DOTRIACONTANE


R.T.: 18.483 min
Delta R.T.: -0.009 min
Response: 135937
Conc: 1.03 ug/ml

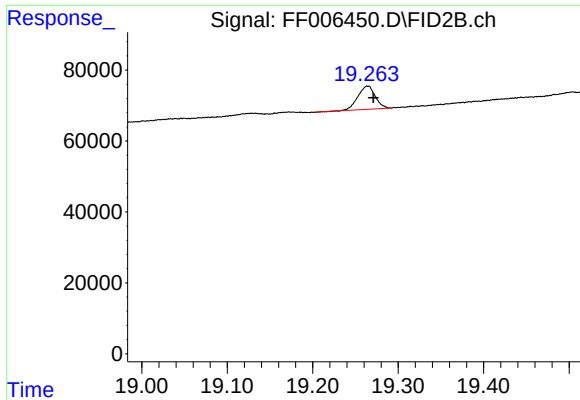

#15 N-TETRATRIACONTANE

R.T.: 19.264 min
Delta R.T.: -0.007 min
Response: 92589
Conc: 0.82 ug/ml

Instrument :
FID_F
ClientSampleId :

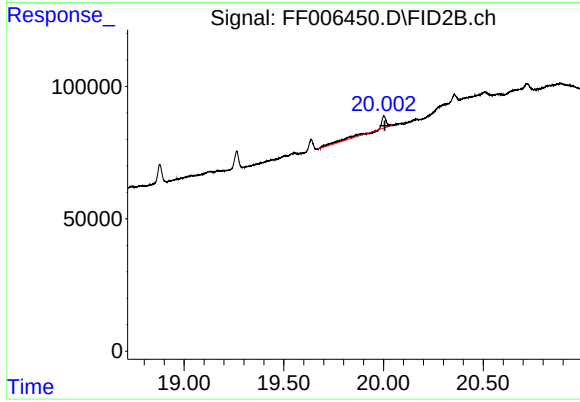

#16 N-HEXATRIACONTANE

R.T.: 20.002 min
Delta R.T.: -0.004 min
Response: 121563
Conc: 1.26 ug/ml