

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
 Data File : FF006452.D
 Signal(s) : FID2B.ch
 Acq On : 21 Feb 2020 20:38
 Operator : DD\AJ
 Sample : L1576-01 5X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 21 22:56:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.604	269962	2.216 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.789	135859	0.972 ug/ml
13) N-TRIACONTANE	17.655	95841	0.693 ug/ml
14) N-DOTRIACONTANE	18.482	144326	1.097 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
Data File : FF006452.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2020 20:38
Operator : DD\AJ
Sample : L1576-01 5X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 22:56:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

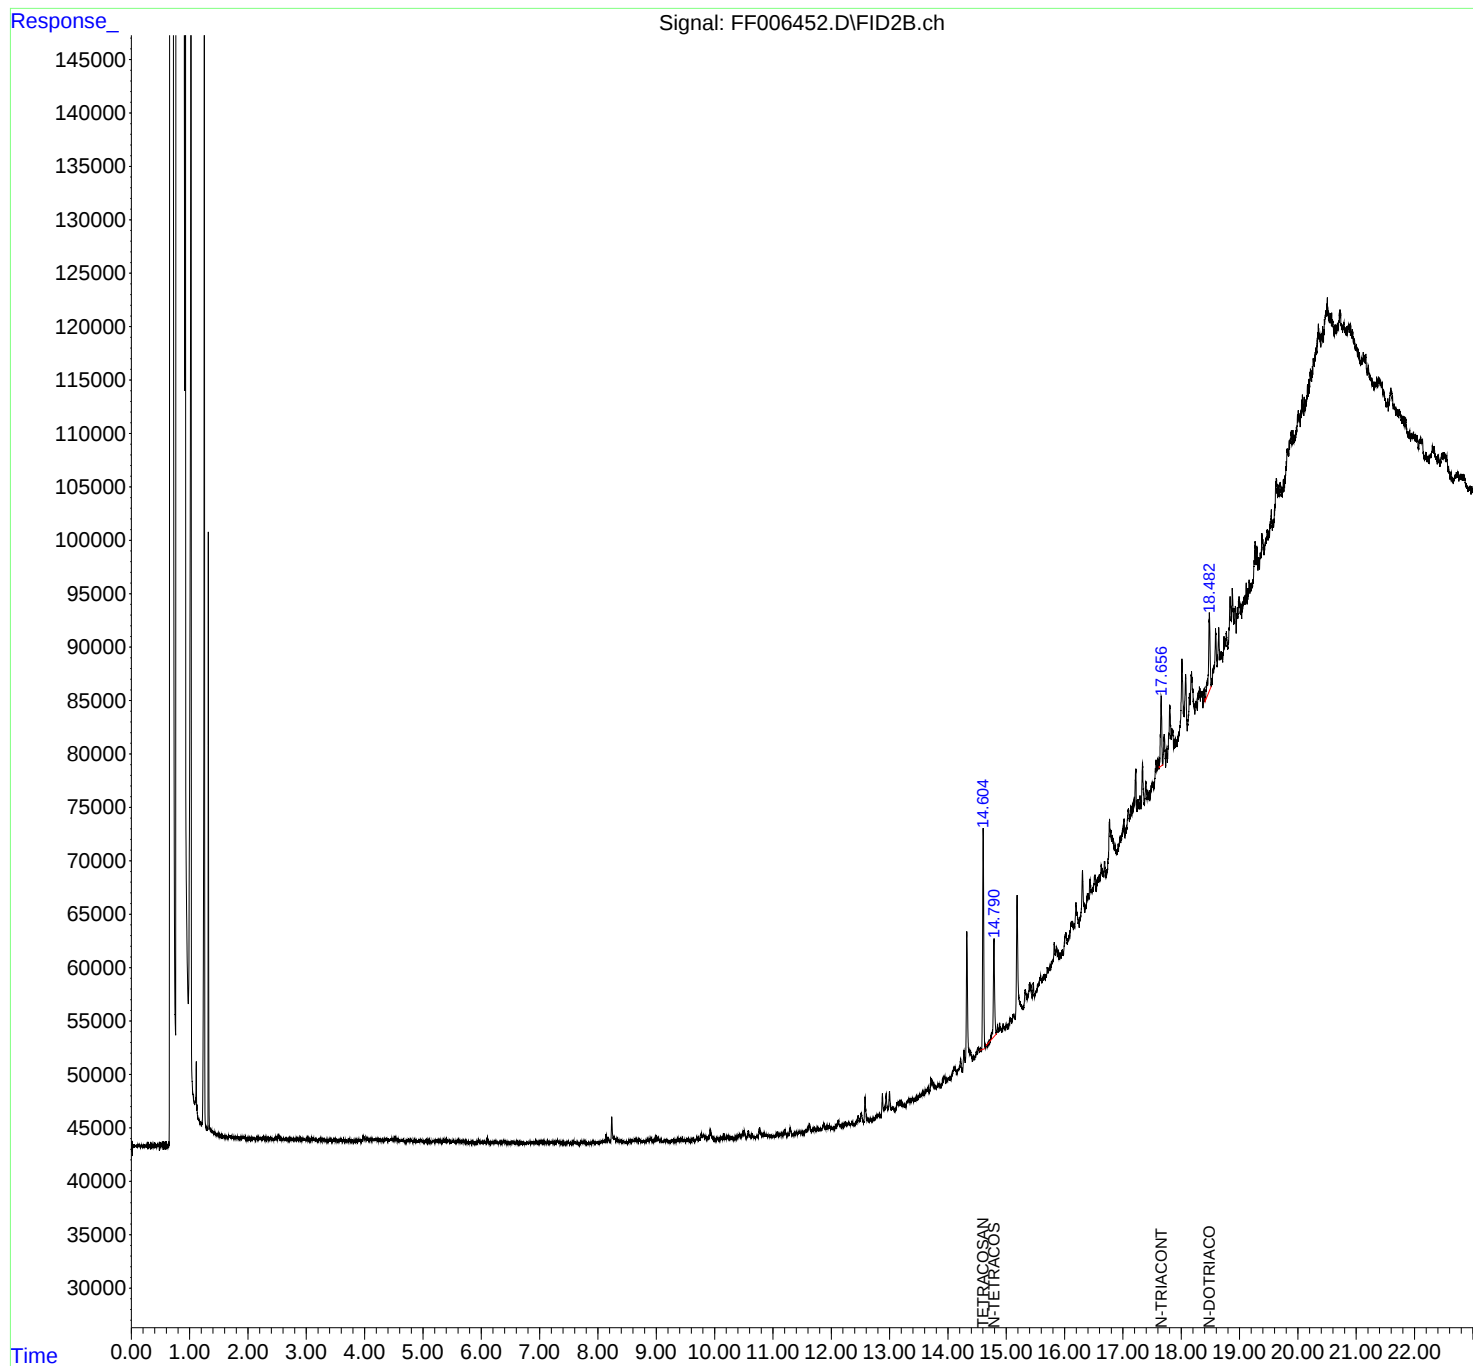


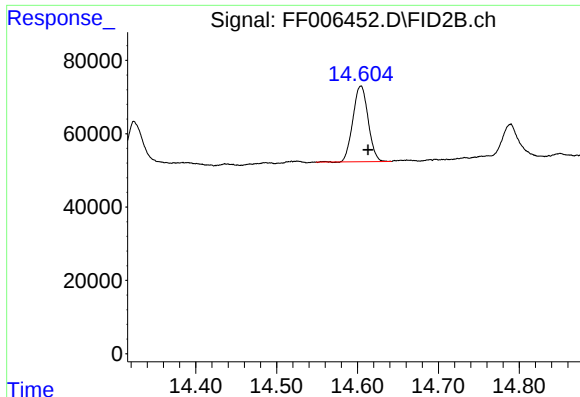

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.604 min
Delta R.T.: -0.009 min
Response: 269962
Conc: 2.22 ug/ml

Instrument :
FID_F
ClientSampleId :

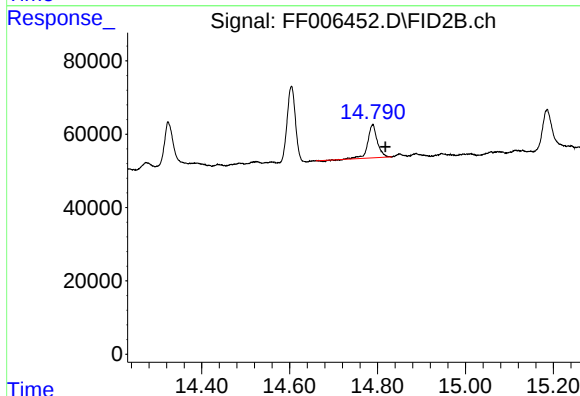


#10 N-TETRACOSANE

R.T.: 14.789 min
Delta R.T.: -0.029 min
Response: 135859
Conc: 0.97 ug/ml

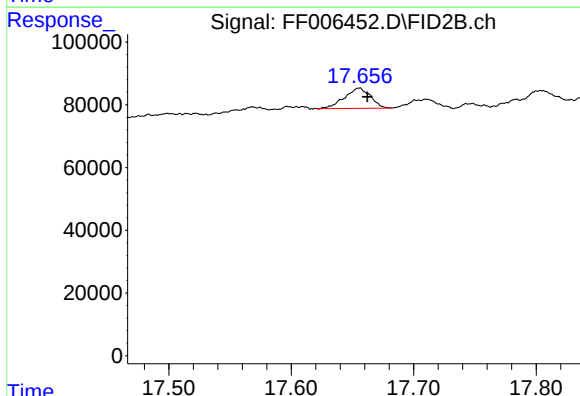

#13 N-TRIACONTANE

R.T.: 17.655 min
Delta R.T.: -0.007 min
Response: 95841
Conc: 0.69 ug/ml

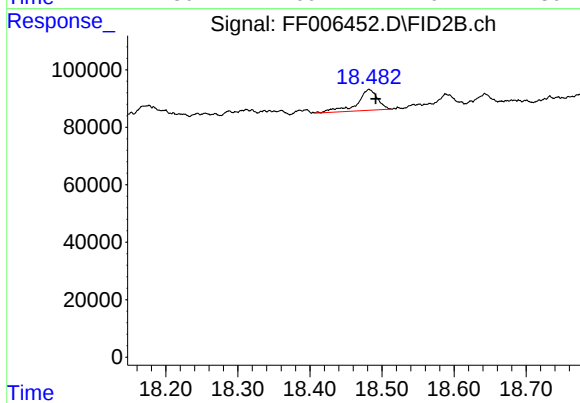

#14 N-DOTRIACONTANE

R.T.: 18.482 min
Delta R.T.: -0.009 min
Response: 144326
Conc: 1.10 ug/ml