

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
 Data File : FF006453.D
 Signal(s) : FID2B.ch
 Acq On : 21 Feb 2020 21:08
 Operator : DD\AJ
 Sample : L1576-02 5X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 21 22:56:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.604	371662	3.051 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.789	142693	1.021 ug/ml
13) N-TRIACONTANE	17.654	164358	1.188 ug/ml
16) N-HEXATRIACONTANE	19.997	3798	0.039 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
Data File : FF006453.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2020 21:08
Operator : DD\AJ
Sample : L1576-02 5X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 21 22:56:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

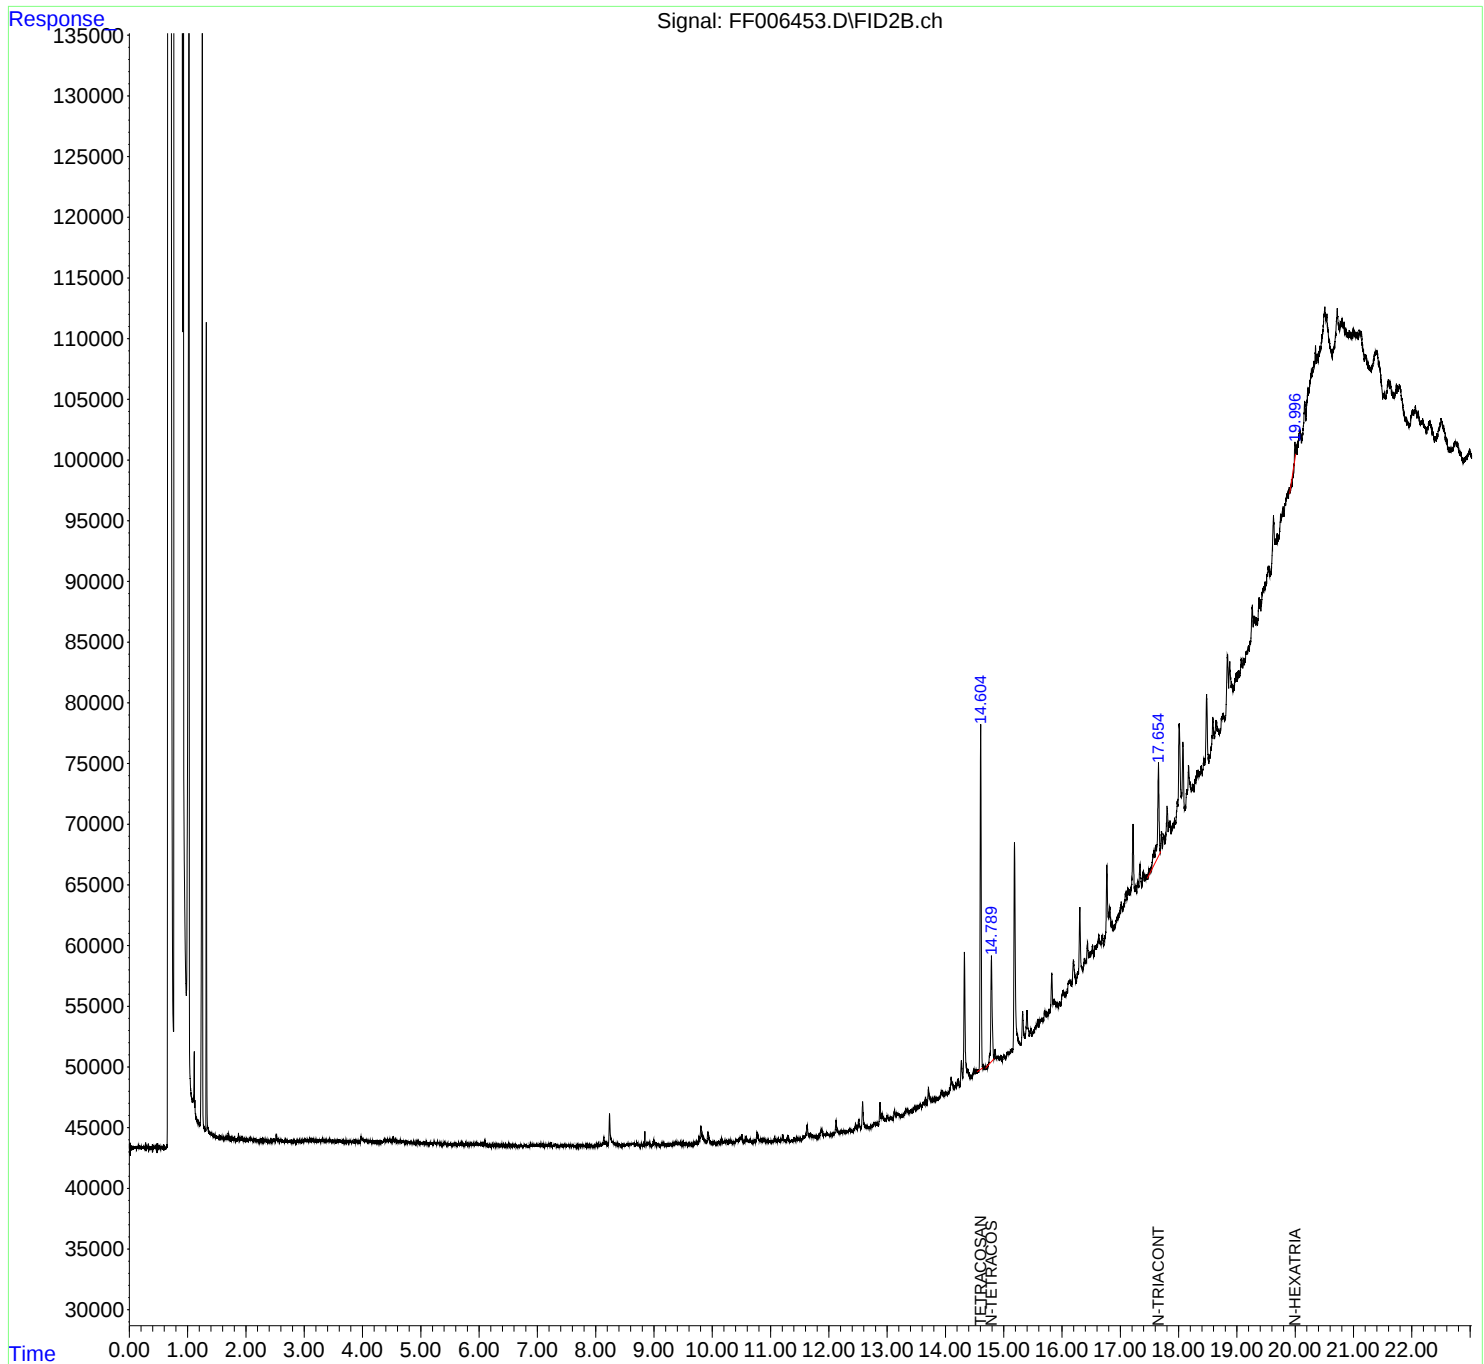


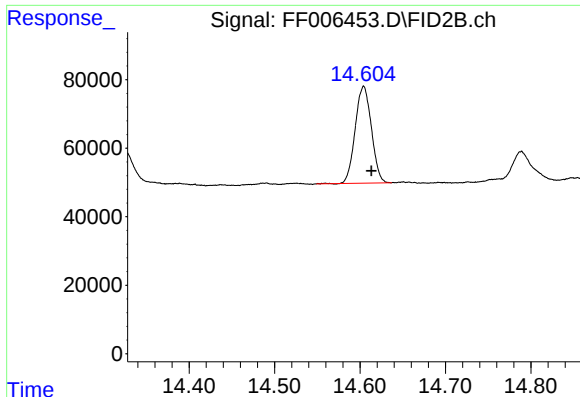

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.604 min
Delta R.T.: -0.009 min
Response: 371662
Conc: 3.05 ug/ml

Instrument :
FID_F
ClientSampleId :

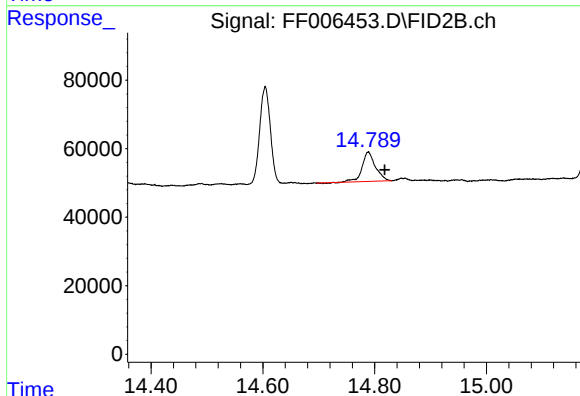


#10 N-TETRACOSANE

R.T.: 14.789 min
Delta R.T.: -0.030 min
Response: 142693
Conc: 1.02 ug/ml

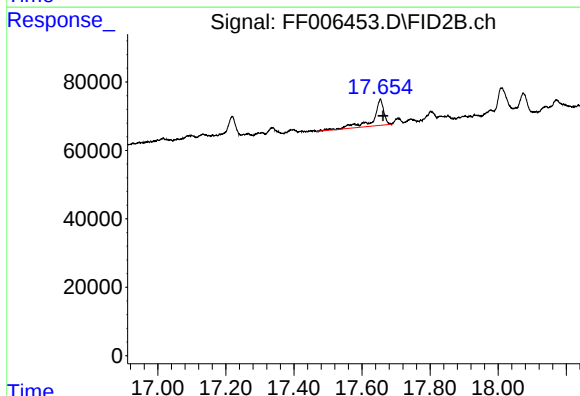

#13 N-TRIACONTANE

R.T.: 17.654 min
Delta R.T.: -0.008 min
Response: 164358
Conc: 1.19 ug/ml

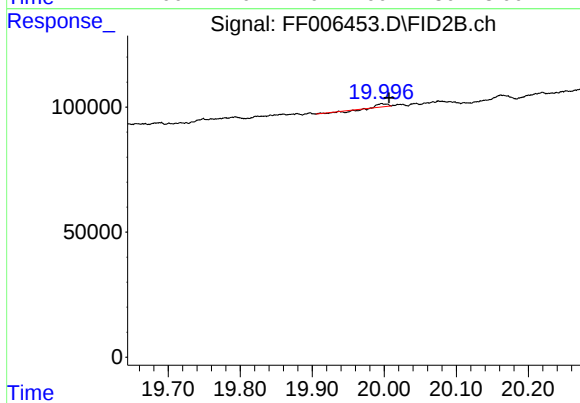

#16 N-HEXATRIACONTANE

R.T.: 19.997 min
Delta R.T.: -0.010 min
Response: 3798
Conc: 0.04 ug/ml