

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
Data File : FF006453.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2020 21:08
Operator : DD\AJ
Sample : L1576-02 5X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WFD-SB-1010203-0-8

Integration File: Sample.e
Quant Time: Feb 21 22:56:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.604	371662	3.051 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022120\
Data File : FF006453.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2020 21:08
Operator : DD\AJ
Sample : L1576-02 5X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
WFD-SB-1010203-0-8

Integration File: Sample.e
Quant Time: Feb 21 22:56:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

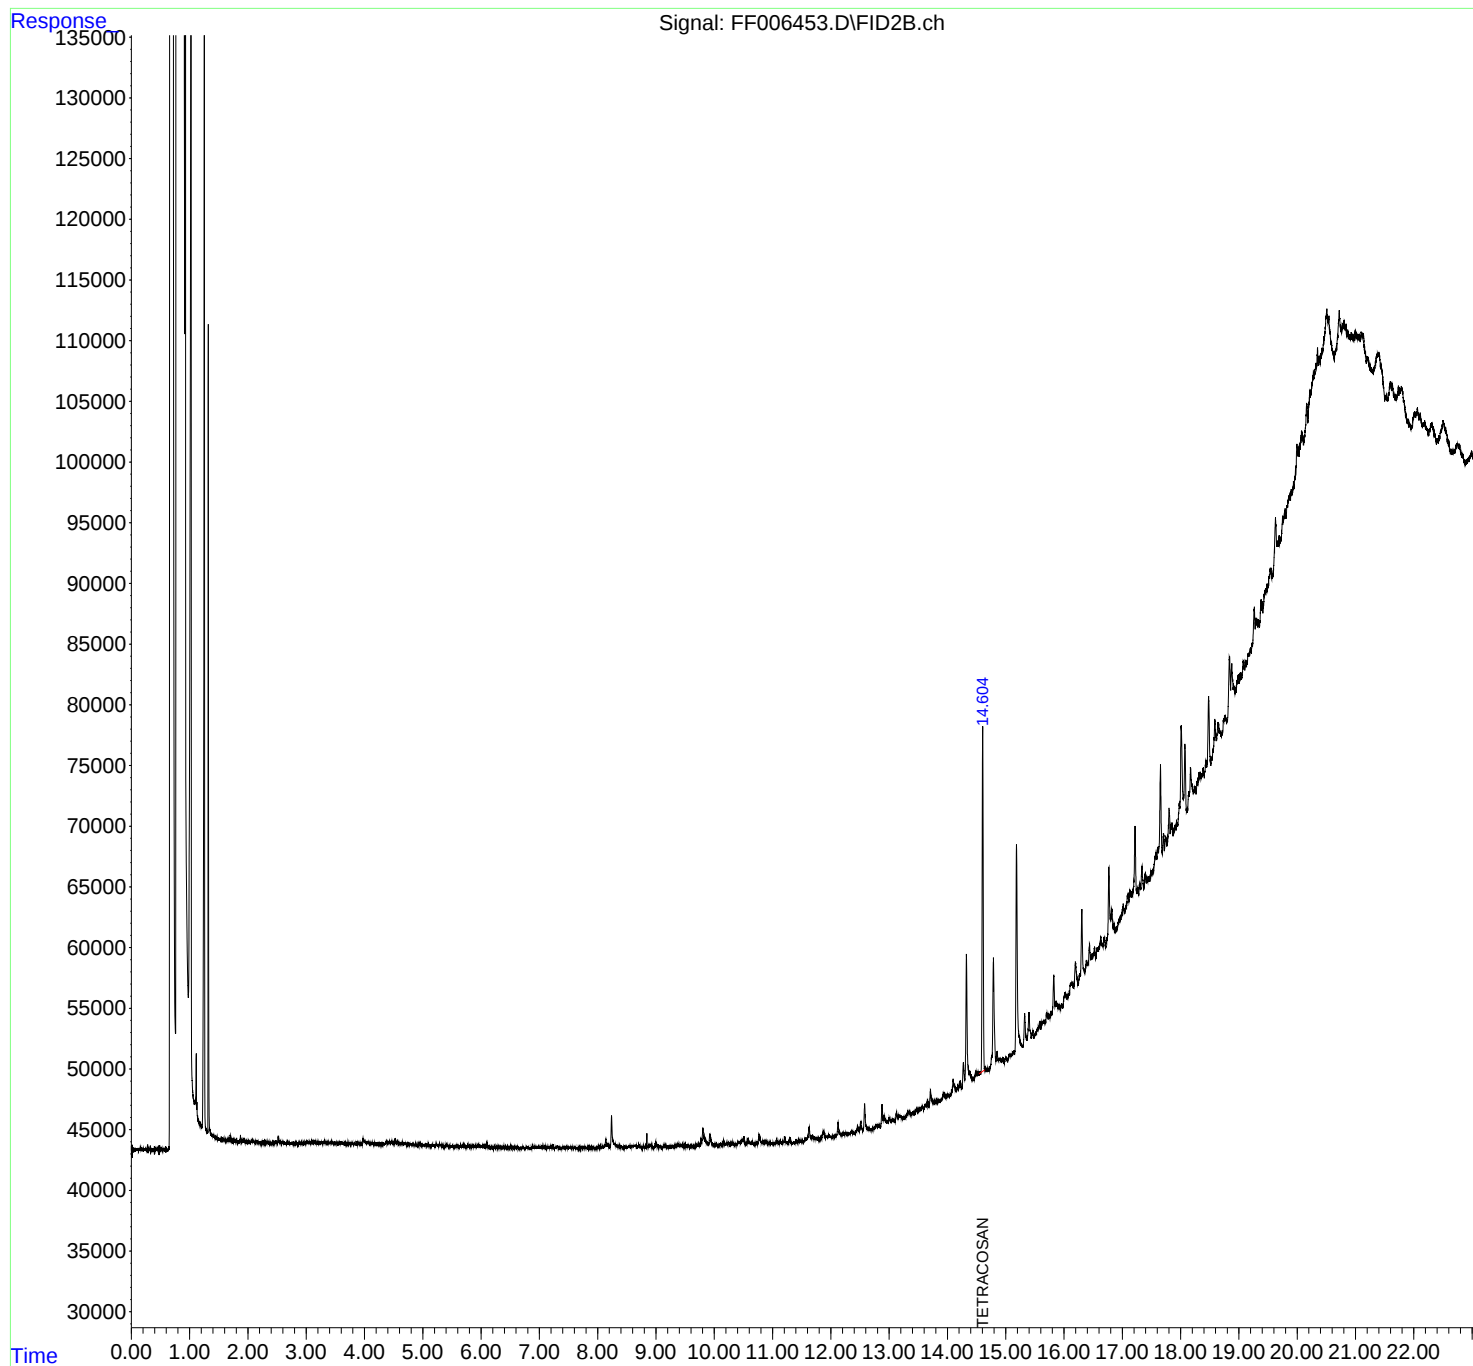

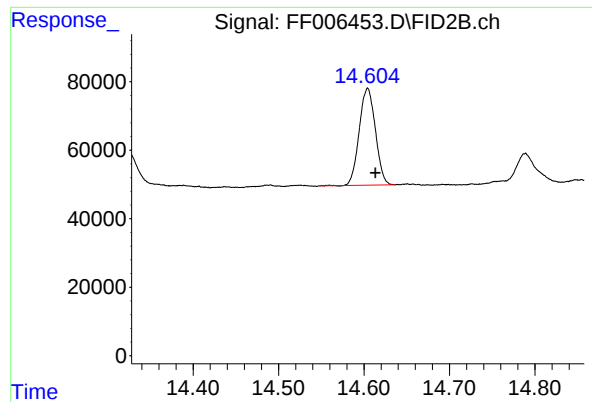

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.604 min
Delta R.T.: -0.009 min
Response: 371662
Conc: 3.05 ug/ml

Instrument :
FID_F
ClientSampleId :
WFD-SB-1010203-0-8