

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022122\
Data File : FF009960.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2022 13:49
Operator : AJ\MA
Sample : PB142825BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 22 00:09:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.412	1942298	17.970 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	19.853	87146	0.828 ug/ml
18) N-TETRACONTANE	21.356	111567	1.201 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022122\
Data File : FF009960.D
Signal(s) : FID2B.ch
Acq On : 21 Feb 2022 13:49
Operator : AJ\MA
Sample : PB142825BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 22 00:09:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

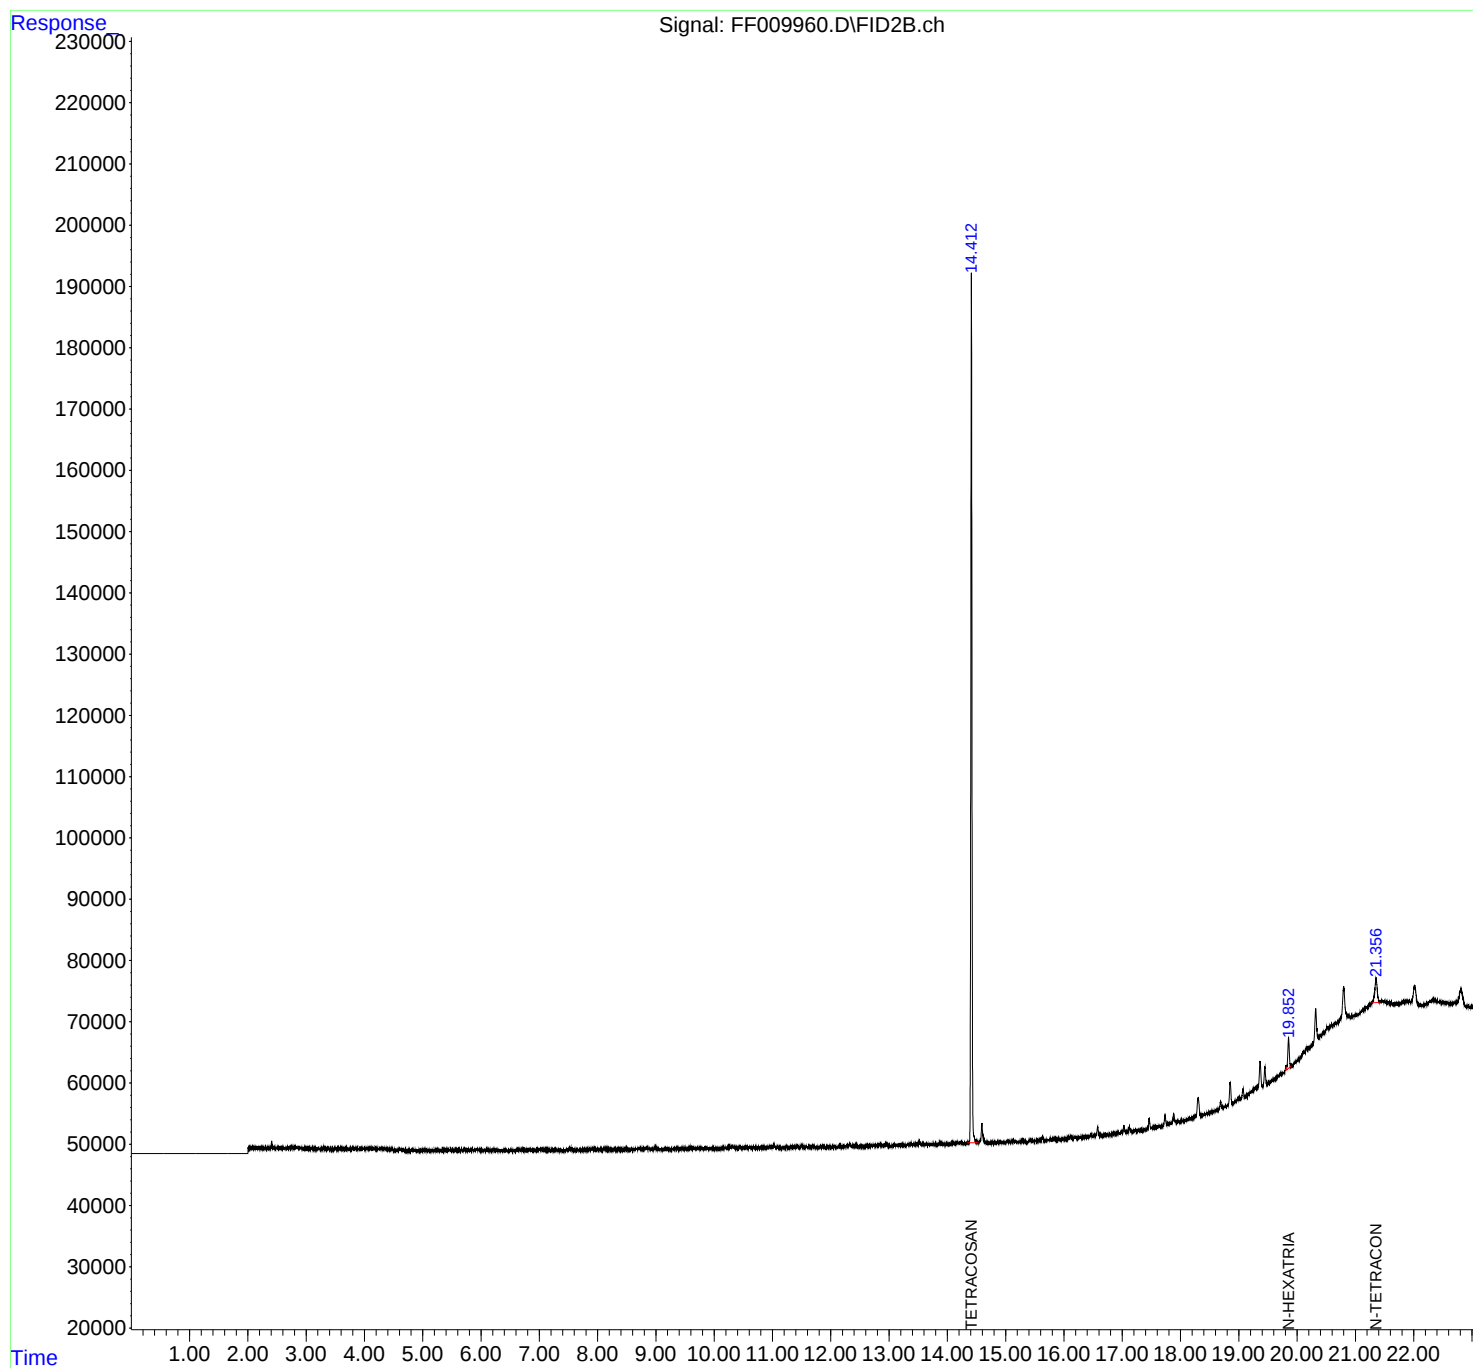


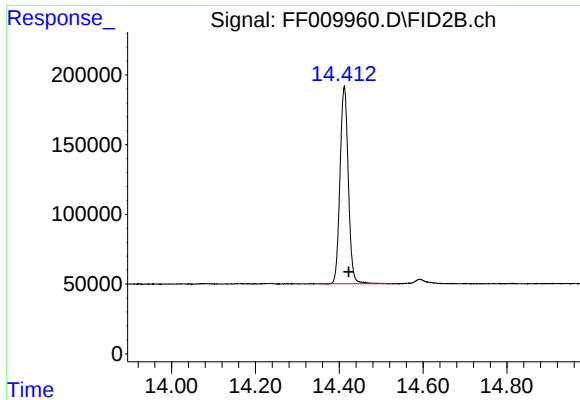

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.412 min
Delta R.T.: -0.010 min
Response: 1942298
Conc: 17.97 ug/ml

Instrument :
FID_F
ClientSampleId :

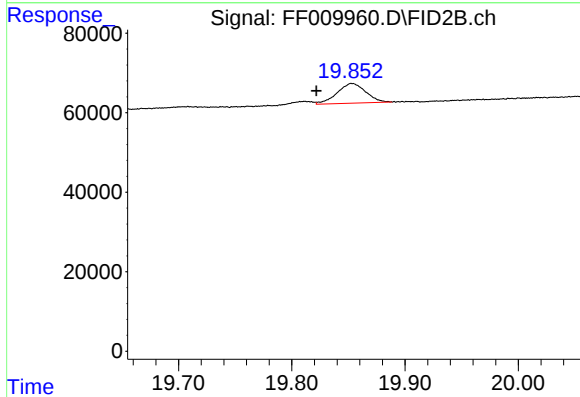

#16 N-HEXATRIACONTANE

R.T.: 19.853 min
Delta R.T.: 0.032 min
Response: 87146
Conc: 0.83 ug/ml

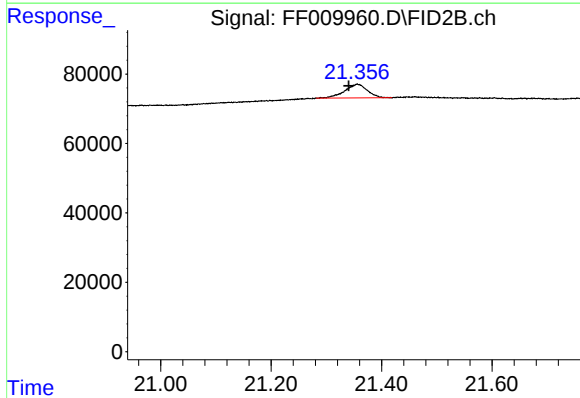

#18 N-TETRACONTANE

R.T.: 21.356 min
Delta R.T.: 0.016 min
Response: 111567
Conc: 1.20 ug/ml