

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022219\
 Data File : FF003606.D
 Signal(s) : FID2B.ch
 Acq On : 22 Feb 2019 15:39
 Operator : AJ\SJ
 Sample : K1556-01MS
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Feb 22 21:48:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
 Quant Title :
 QLast Update : Fri Feb 01 22:57:49 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.606	2386138	19.765 ug/mlm
Target Compounds			
2) N-DECANE	4.332	2050800	15.324 ug/ml
3) N-DODECANE	6.354	2292747	17.005 ug/ml
4) N-TETRADECANE	8.146	2346895	17.339 ug/mlm
5) N-HEXADECANE	9.748	2453417	18.003 ug/ml
6) N-OCTADECANE	11.191	2350532	17.082 ug/mlm
7) N-EICOSANE	12.504	2363792	17.189 ug/mlm
8) N-DOCOSANE	13.702	2685324	19.627 ug/mlm
10) N-TETRACOSANE	14.809	2101751	15.455 ug/mlm
11) N-HEXACOSANE	15.836	2608410	19.231 ug/ml
12) N-OCTACOSANE	16.790	3439767	25.123 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022219\
Data File : FF003606.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2019 15:39
Operator : AJ\SJ
Sample : K1556-01MS
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Feb 22 21:48:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF020119.M
Quant Title :
QLast Update : Fri Feb 01 22:57:49 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

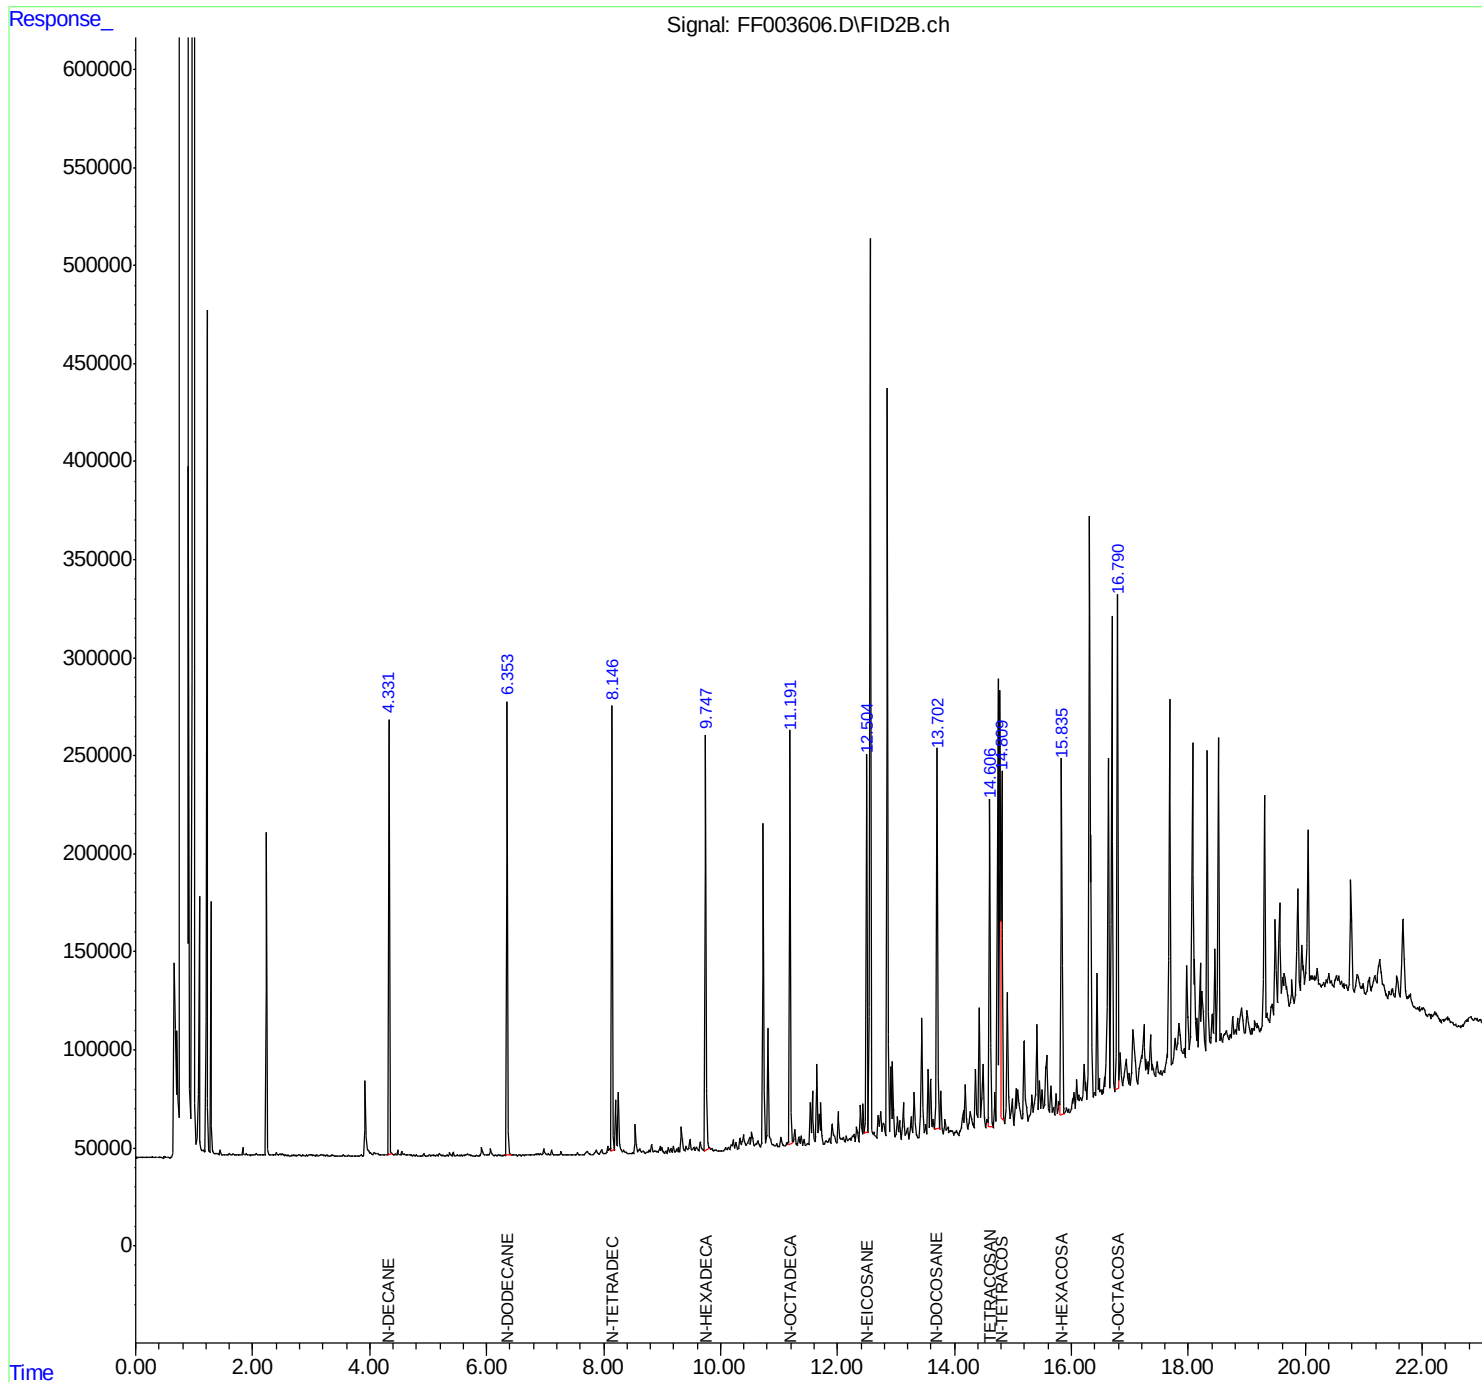

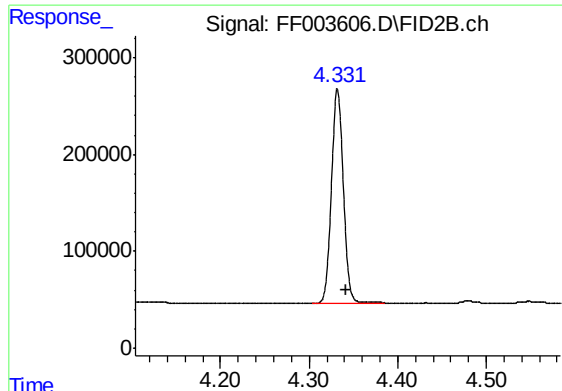


#2 N-DECANE

R.T.: 4.332 min
Delta R.T.: -0.010 min
Response: 2050800
Conc: 15.32 ug/ml

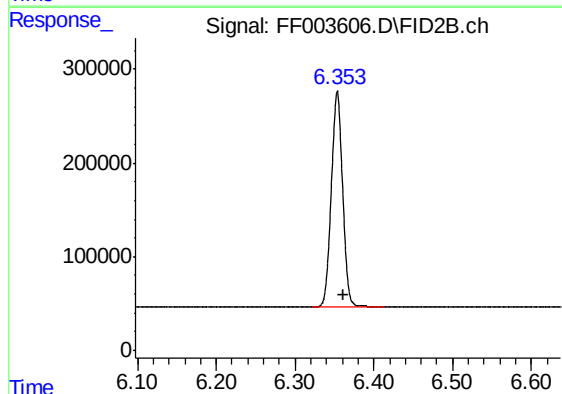


#3 N-DODECANE

R.T.: 6.354 min
Delta R.T.: -0.007 min
Response: 2292747
Conc: 17.00 ug/ml

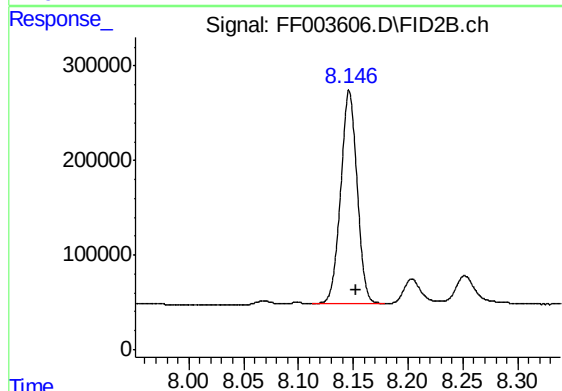


#4 N-TETRADECANE

R.T.: 8.146 min
Delta R.T.: -0.008 min
Response: 2346895
Conc: 17.34 ug/ml m

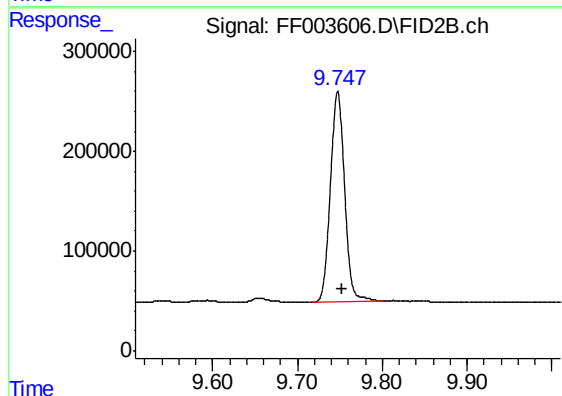


#5 N-HEXADECANE

R.T.: 9.748 min
Delta R.T.: -0.005 min
Response: 2453417
Conc: 18.00 ug/ml

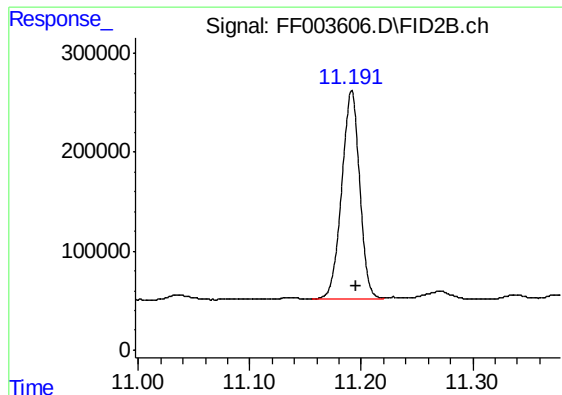


#6 N-OCTADECANE

R.T.: 11.191 min
Delta R.T.: -0.004 min
Response: 2350532
Conc: 17.08 ug/ml m

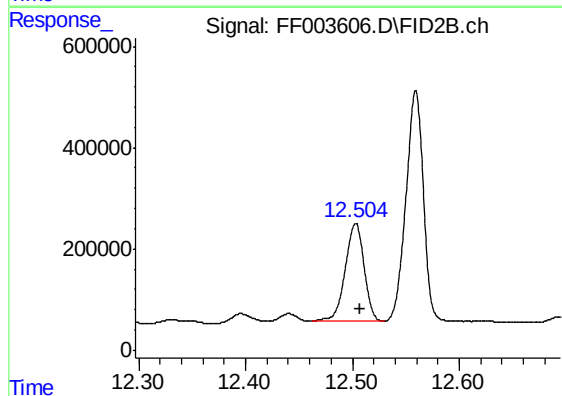


#7 N-EICOSANE

R.T.: 12.504 min
Delta R.T.: -0.004 min
Response: 2363792
Conc: 17.19 ug/ml m

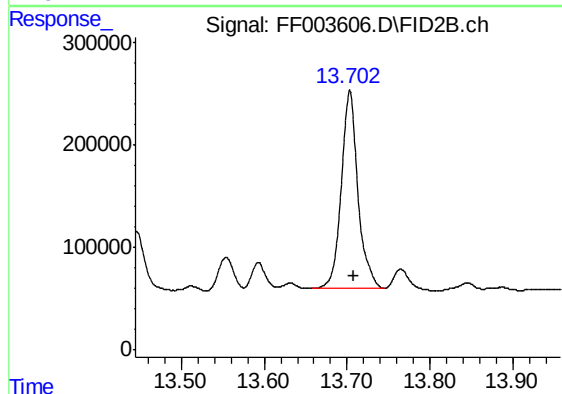


#8 N-DOCOSANE

R.T.: 13.702 min
Delta R.T.: -0.005 min
Response: 2685324
Conc: 19.63 ug/ml m

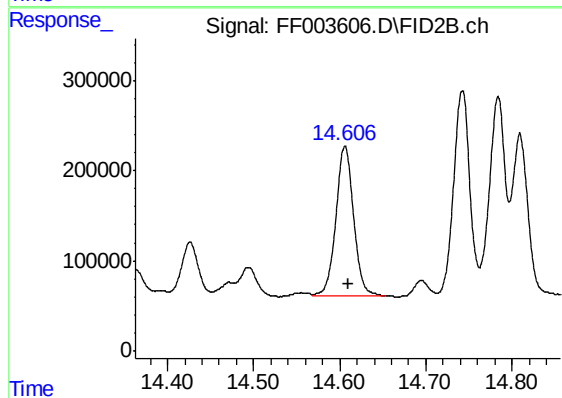


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.606 min
Delta R.T.: -0.004 min
Response: 2386138
Conc: 19.76 ug/ml m

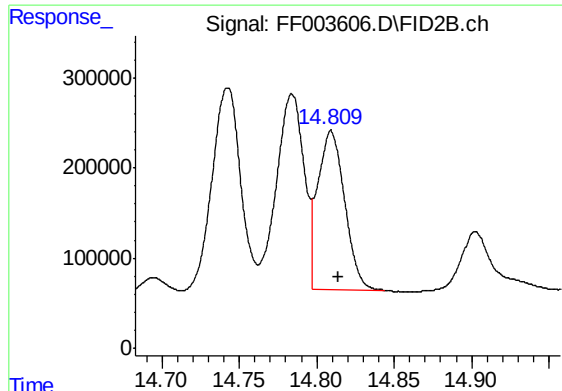


#10 N-TETRACOSANE

R.T.: 14.809 min
Delta R.T.: -0.005 min
Response: 2101751
Conc: 15.45 ug/ml m

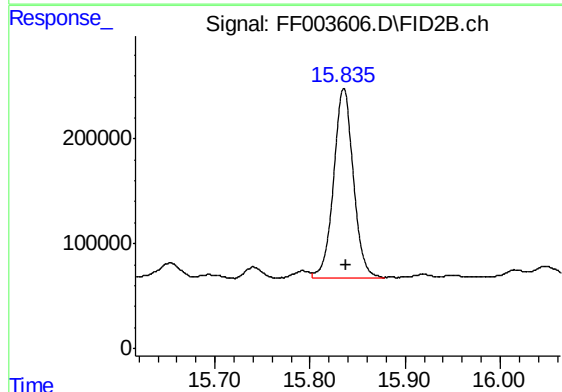

#11 N-HEXACOSANE

R.T.: 15.836 min
Delta R.T.: -0.003 min
Response: 2608410
Conc: 19.23 ug/ml

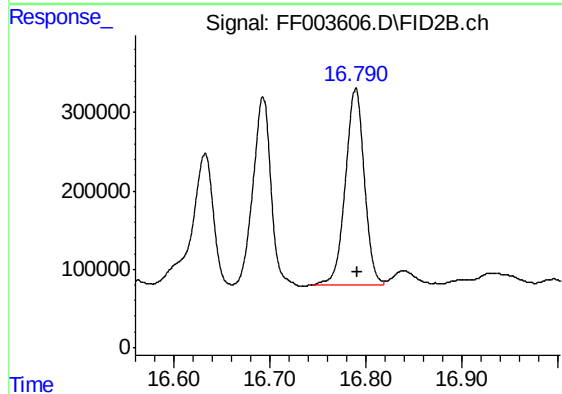

#12 N-OCTACOSANE

R.T.: 16.790 min
Delta R.T.: -0.002 min
Response: 3439767
Conc: 25.12 ug/ml m