

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022222\
Data File : FF009972.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2022 16:52
Operator : AJ\MA
Sample : PB142868BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 00:40:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.412	2532846	23.434 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	19.853	55671	0.529 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022222\
Data File : FF009972.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2022 16:52
Operator : AJ\MA
Sample : PB142868BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 00:40:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

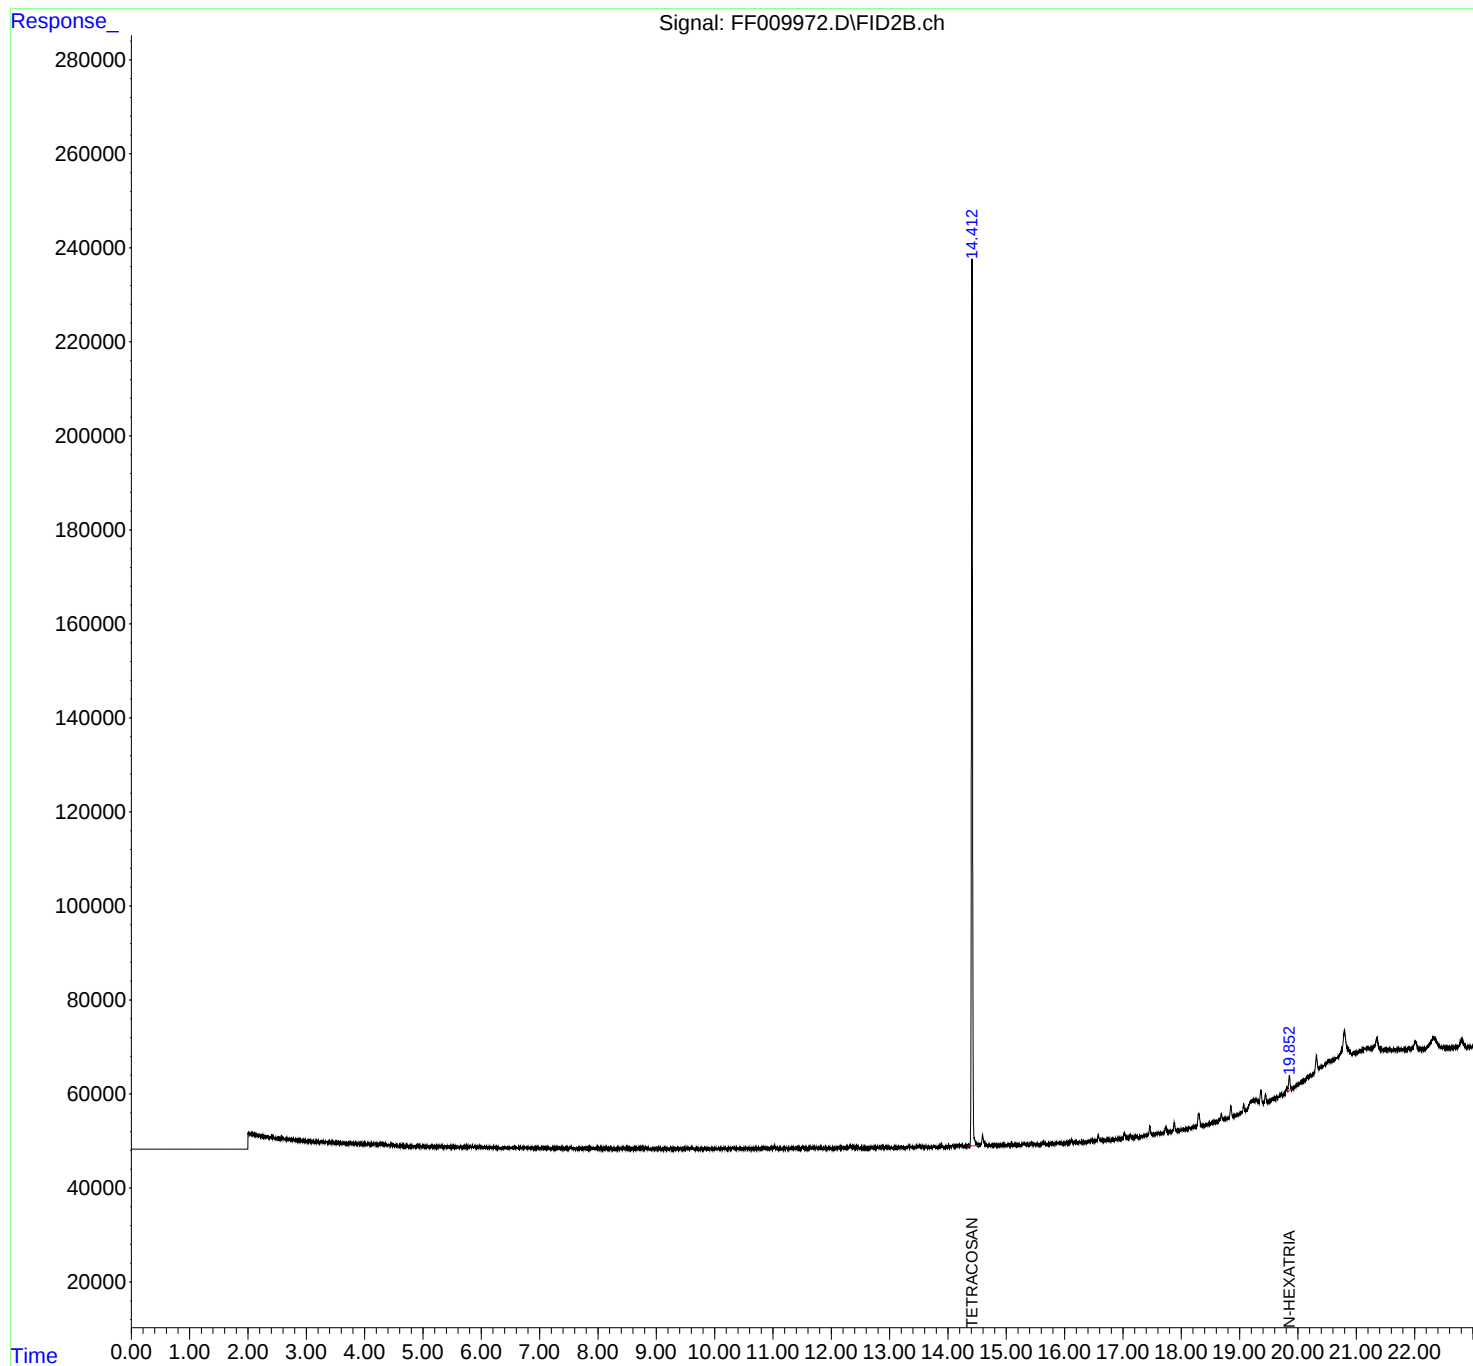


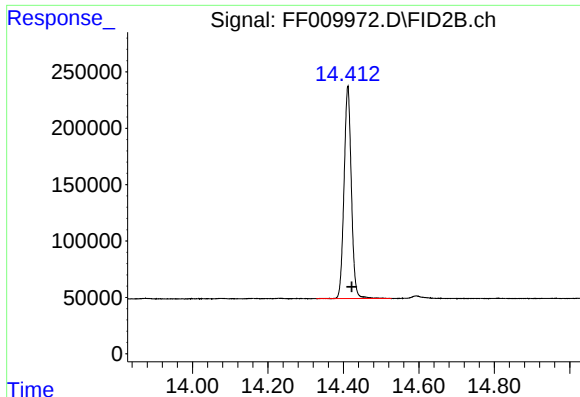

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.412 min
Delta R.T.: -0.010 min
Response: 2532846
Conc: 23.43 ug/ml

Instrument :
FID_F
ClientSampleId :

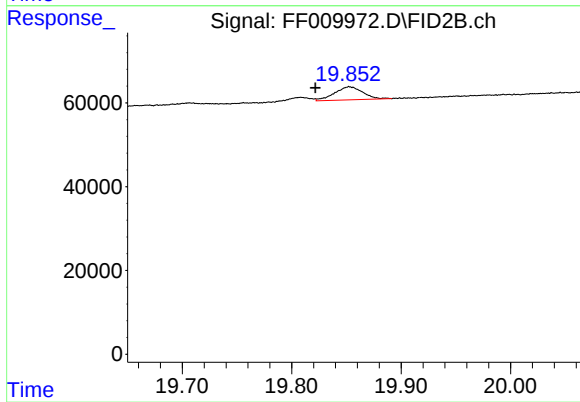

#16 N-HEXATRIACONTANE

R.T.: 19.853 min
Delta R.T.: 0.031 min
Response: 55671
Conc: 0.53 ug/ml