

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022222\
Data File : FF009977.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2022 19:25
Operator : AJ\MA
Sample : N1628-01 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
BP-3

Integration File: autoint1.e
Quant Time: Feb 23 00:41:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.416	224518	2.077 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022222\
Data File : FF009977.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2022 19:25
Operator : AJ\MA
Sample : N1628-01 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
BP-3

Integration File: autoint1.e
Quant Time: Feb 23 00:41:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021022.M
Quant Title :
QLast Update : Fri Feb 11 12:58:22 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

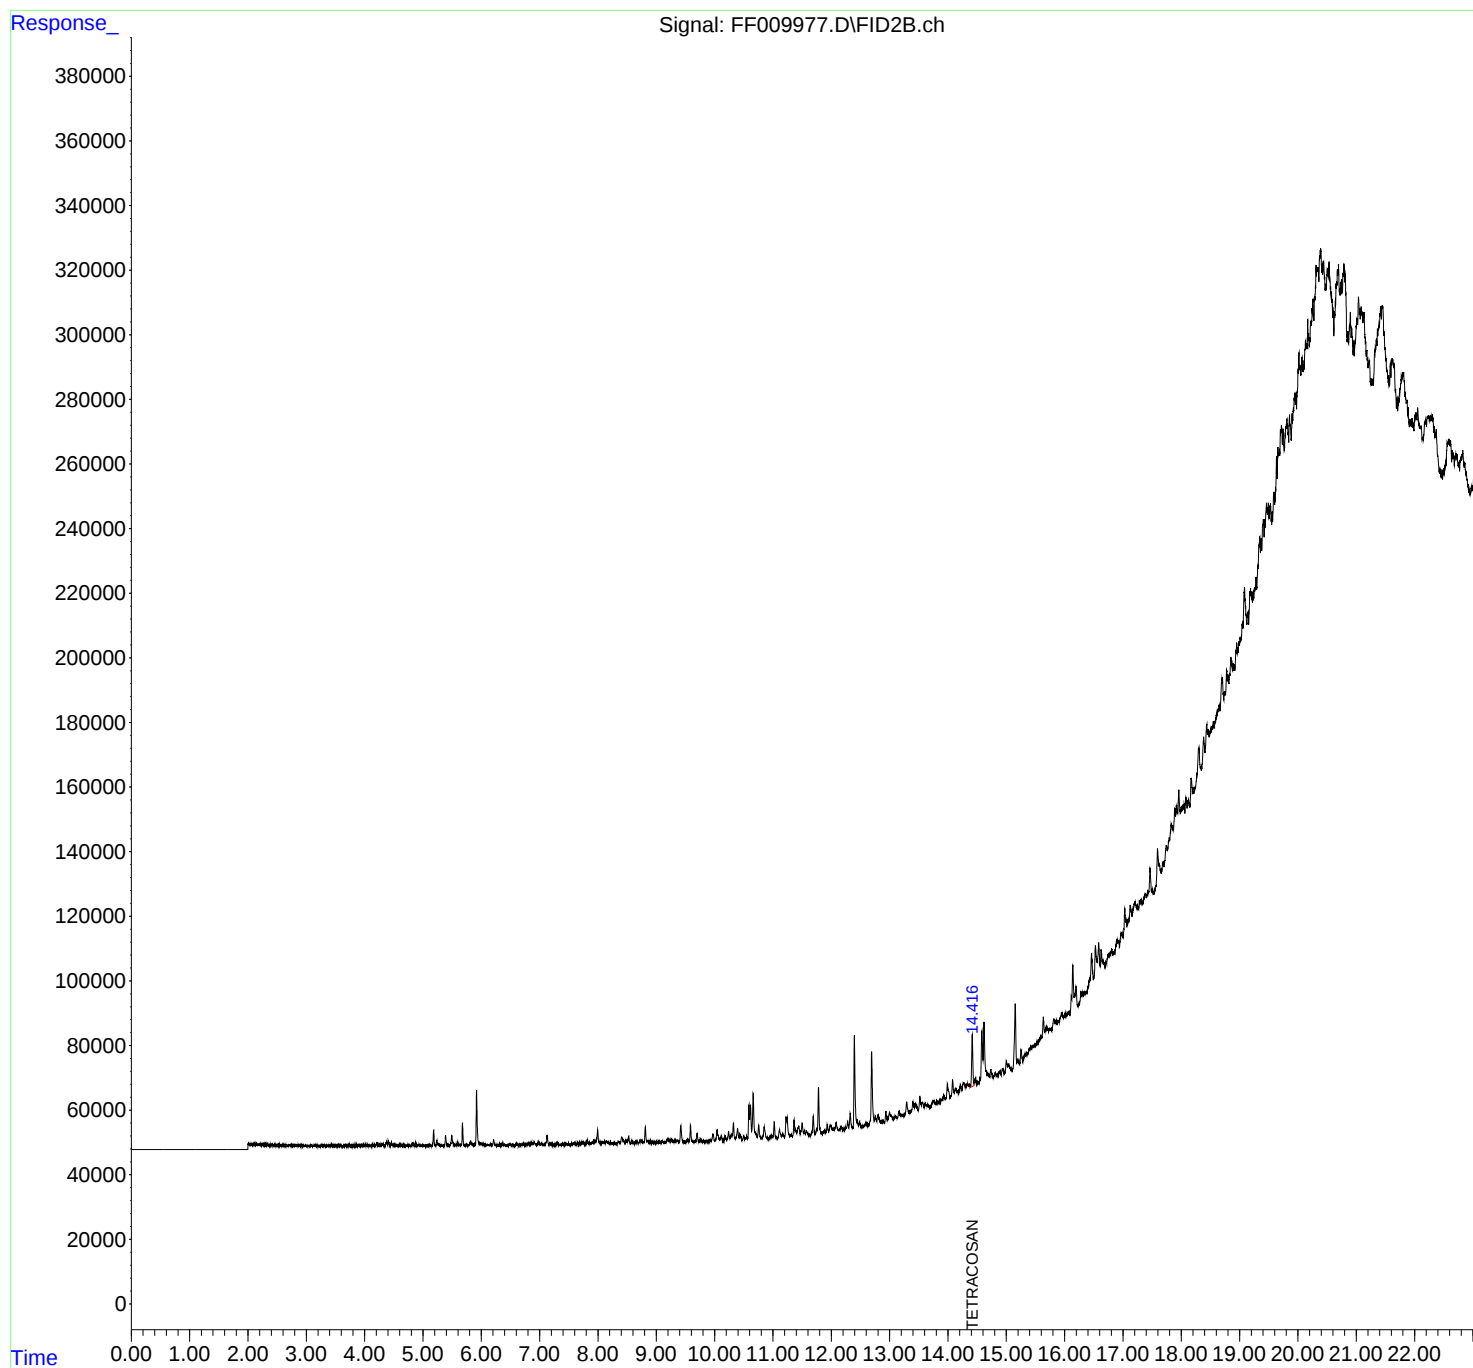

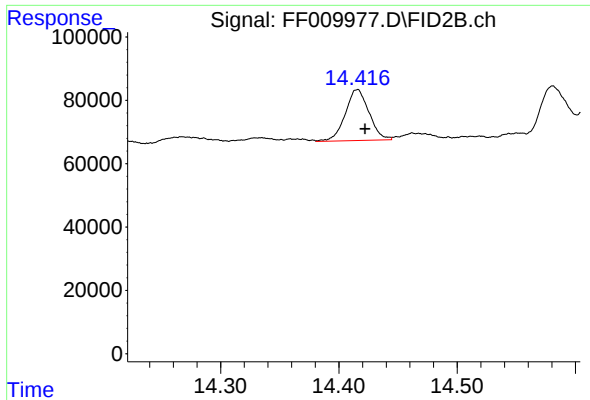

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.416 min
Delta R.T.: -0.007 min
Response: 224518
Conc: 2.08 ug/ml

Instrument :

FID_F

ClientSampleId :

BP-3