

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
 Data File : FF012174.D
 Signal(s) : FID2B.ch
 Acq On : 22 Feb 2023 08:24
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 23 00:48:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:12:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.959	97427	0.691 ug/ml
10) N-TETRACOSANE	15.236	89673	0.677 ug/ml
12) N-OCTACOSANE	17.212	107089	0.872 ug/ml
13) N-TRIACONTANE	18.102	74317	0.637 ug/ml
14) N-DOTRIACONTANE	18.936	494145	4.438 ug/ml
15) N-TETRATRIACONTANE	19.718	65764	0.665 ug/ml
16) N-HEXATRIACONTANE	20.486	354124	3.734 ug/ml
18) N-TETRACONTANE	22.139	263601	2.895 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012174.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 08:24
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 00:48:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

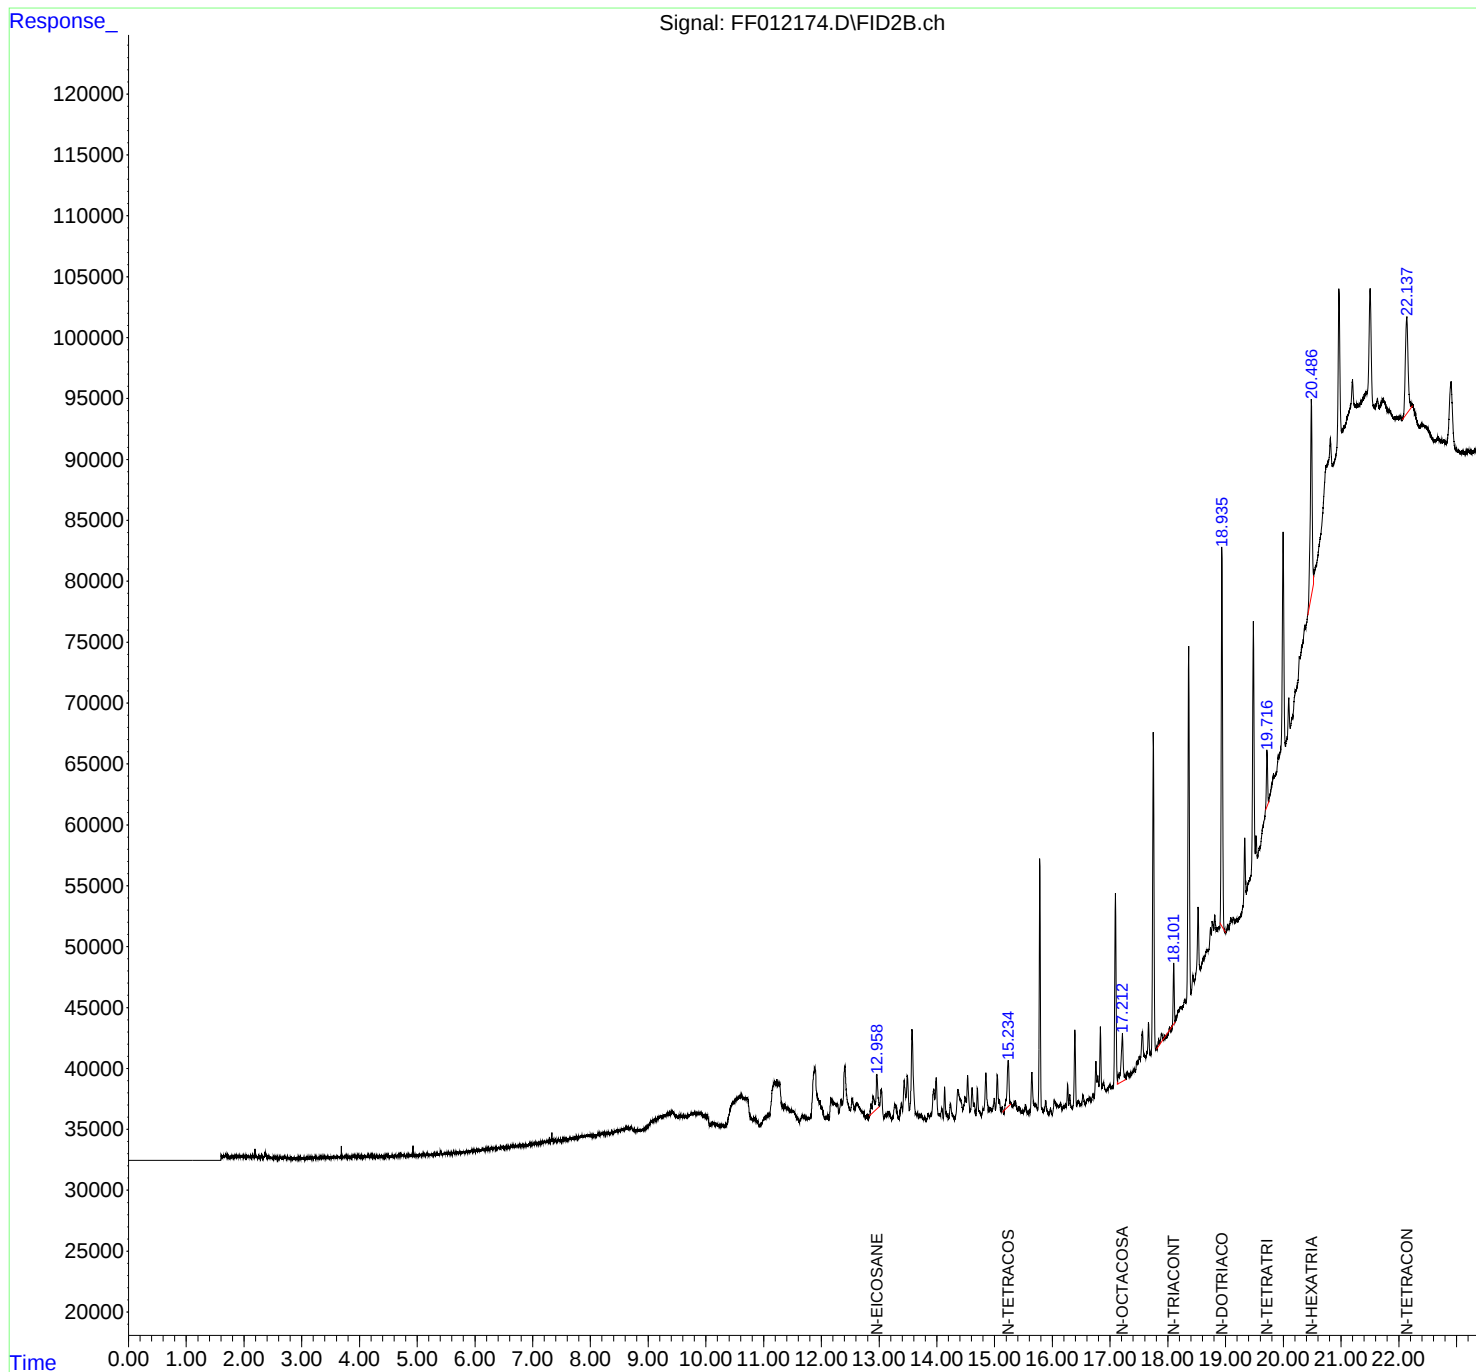


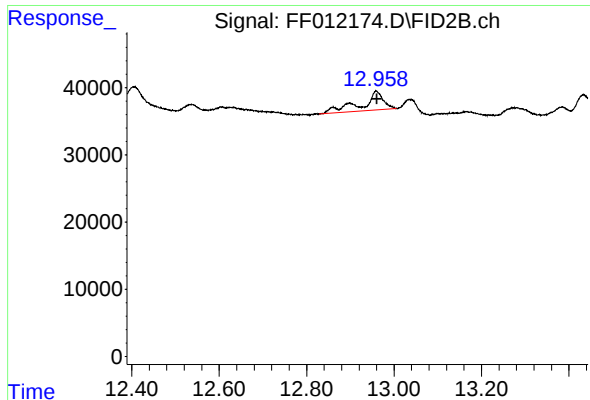

#7 N-EICOSANE


R.T.: 12.959 min
Delta R.T.: -0.002 min
Response: 97427
Conc: 0.69 ug/ml

Instrument :
FID_F
ClientSampleId :

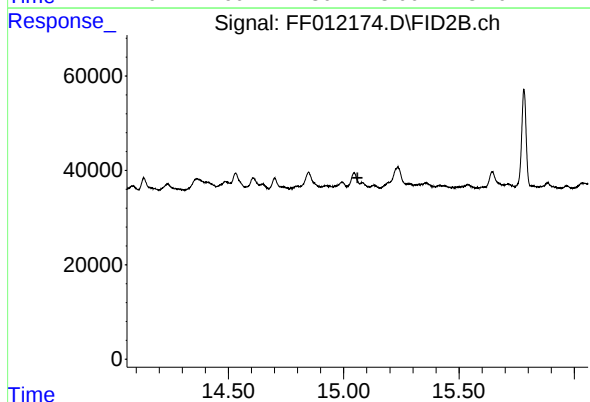


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.060 min
Response: 0
Conc: N.D.

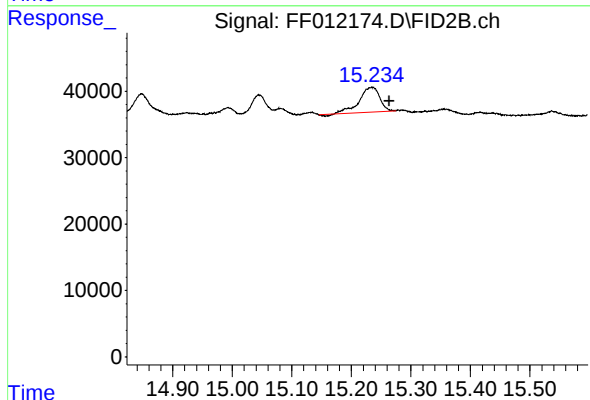


#10 N-TETRACOSANE

R.T.: 15.236 min
Delta R.T.: -0.029 min
Response: 89673
Conc: 0.68 ug/ml

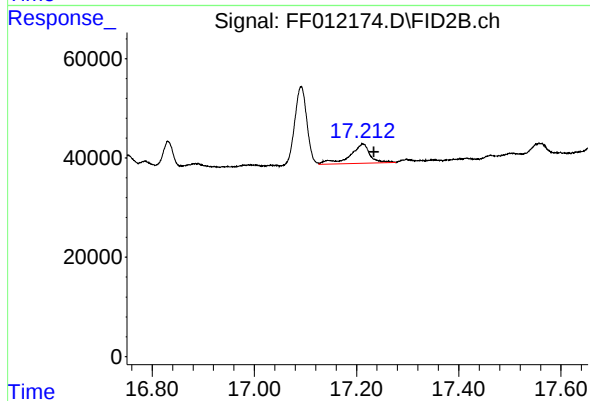

#12 N-OCTACOSANE


R.T.: 17.212 min
Delta R.T.: -0.022 min
Response: 107089
Conc: 0.87 ug/ml

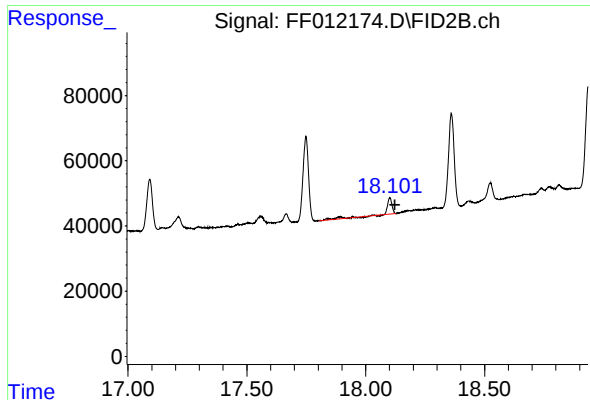

#13 N-TRIACONTANE


R.T.: 18.102 min
Delta R.T.: -0.020 min
Response: 74317
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

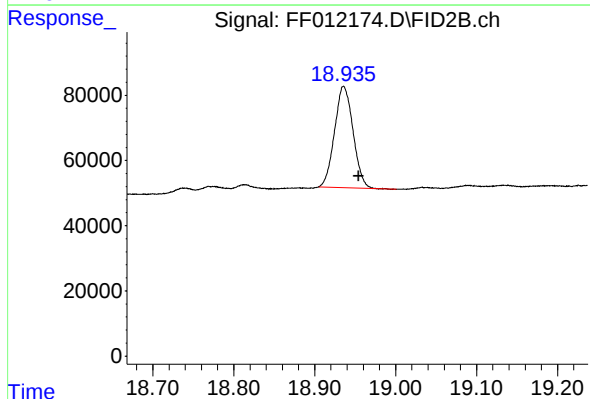


#14 N-DOTRIACONTANE

R.T.: 18.936 min
Delta R.T.: -0.019 min
Response: 494145
Conc: 4.44 ug/ml

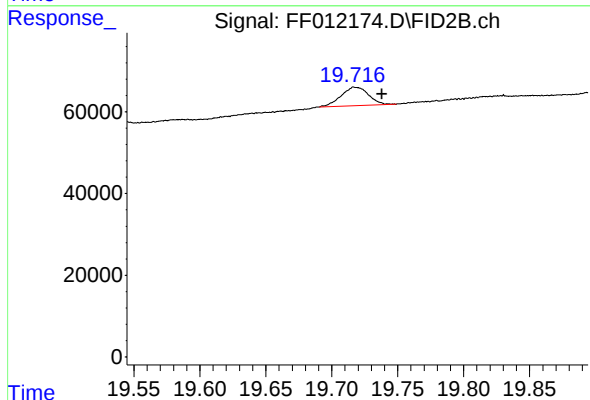


#15 N-TETRATRIACONTANE

R.T.: 19.718 min
Delta R.T.: -0.020 min
Response: 65764
Conc: 0.66 ug/ml

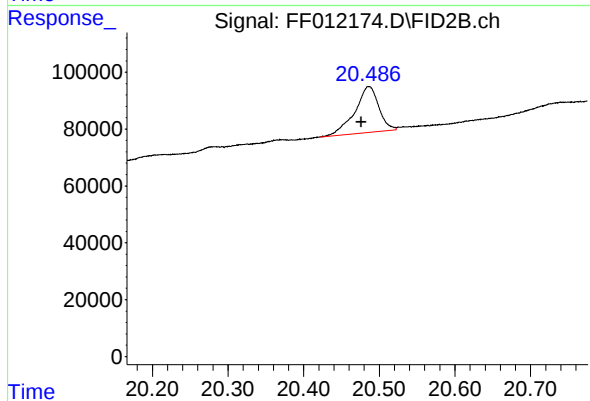

#16 N-HEXATRIACONTANE

R.T.: 20.486 min
Delta R.T.: 0.010 min
Response: 354124
Conc: 3.73 ug/ml

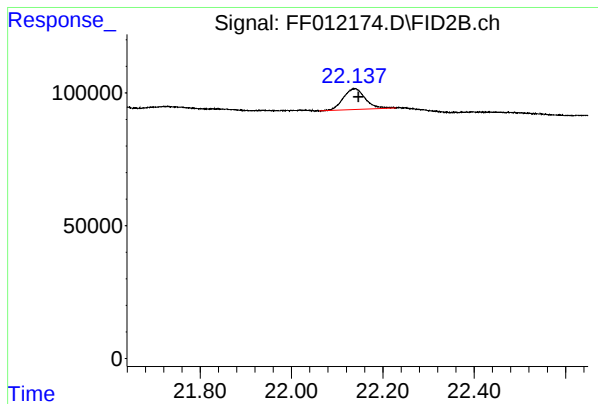

#18 N-TETRACONTANE

R.T.: 22.139 min
Delta R.T.: -0.008 min
Response: 263601
Conc: 2.89 ug/ml

Instrument :
FID_F
ClientSampleId :