

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
 Data File : FF012177.D
 Signal(s) : FID2B.ch
 Acq On : 22 Feb 2023 09:51
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 23 00:49:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:12:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.762	2208085	16.253 ug/ml
12) N-OCTACOSANE	17.218	2285196	18.618 ug/ml
14) N-DOTRIACONTANE	18.939	106479	0.956 ug/ml
16) N-HEXATRIACONTANE	20.488	144065	1.519 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012177.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 09:51
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 00:49:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

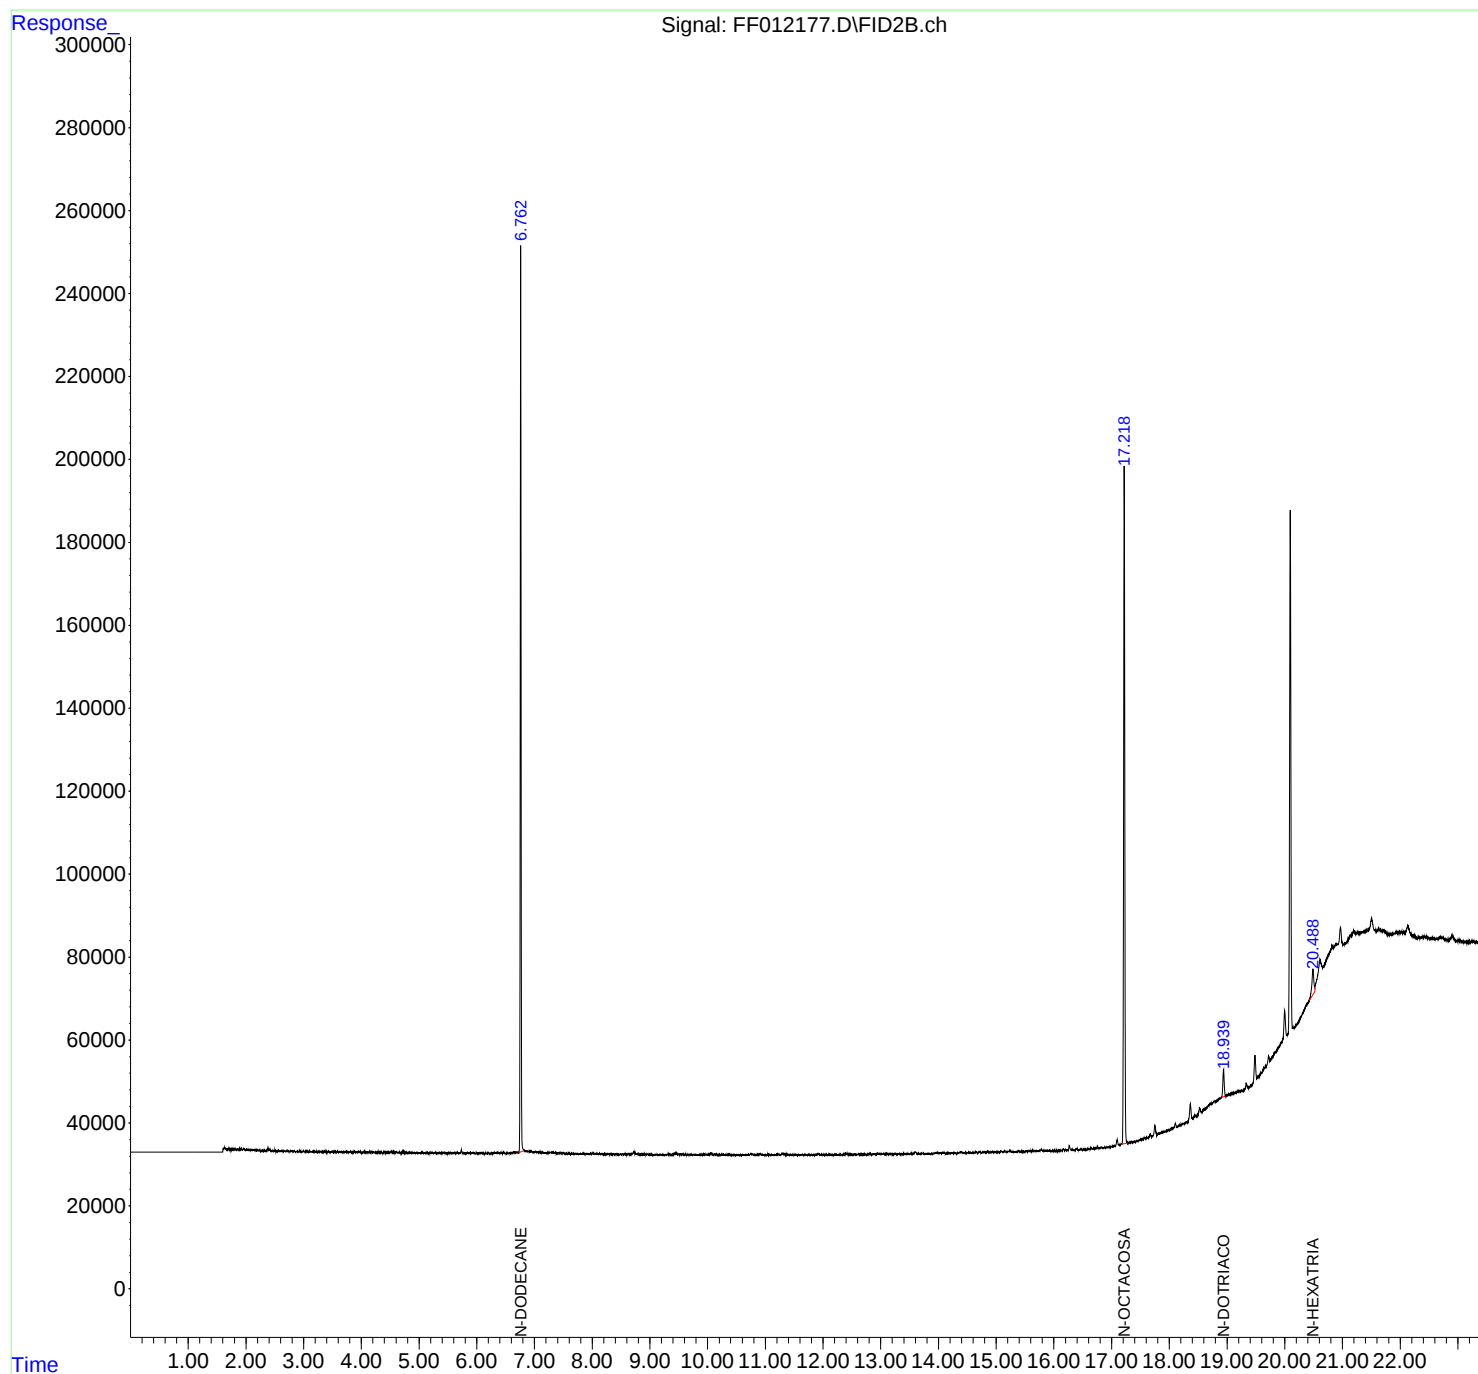


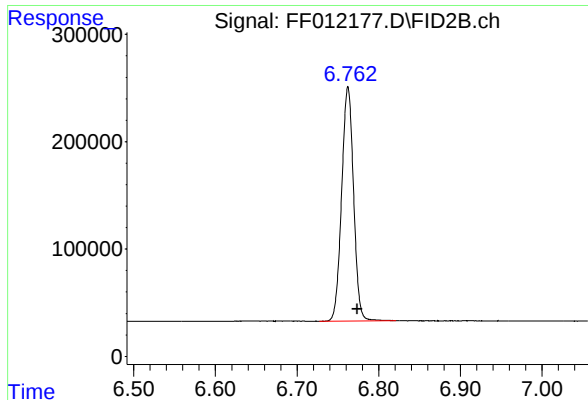

#3 N-DODECANE


R.T.: 6.762 min
Delta R.T.: -0.011 min
Response: 2208085
Conc: 16.25 ug/ml

Instrument :
FID_F
ClientSampleId :

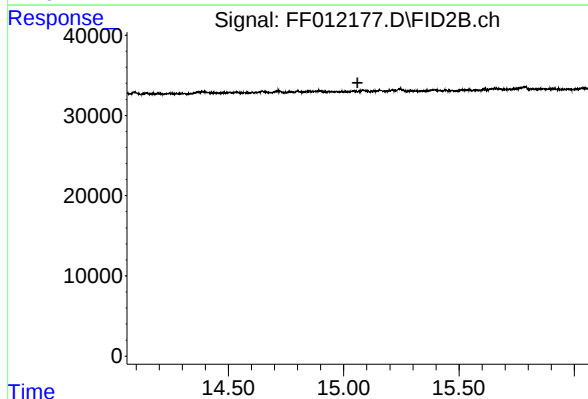


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.060 min
Response: 0
Conc: N.D.

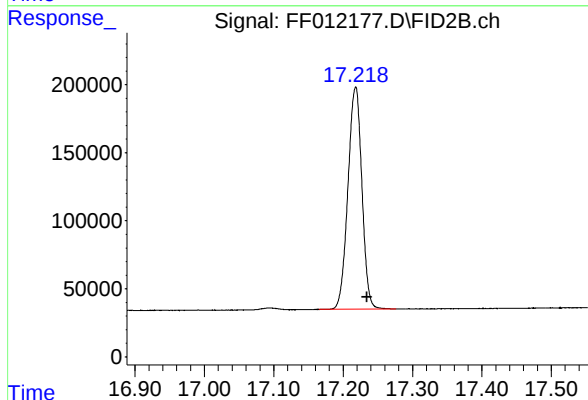


#12 N-OCTACOSANE

R.T.: 17.218 min
Delta R.T.: -0.016 min
Response: 2285196
Conc: 18.62 ug/ml

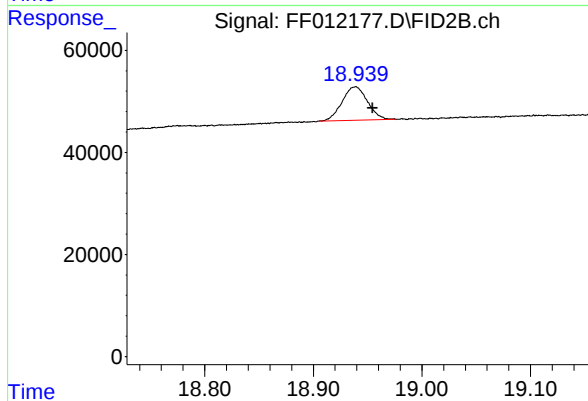

#14 N-DOTRIACONTANE

R.T.: 18.939 min
Delta R.T.: -0.016 min
Response: 106479
Conc: 0.96 ug/ml

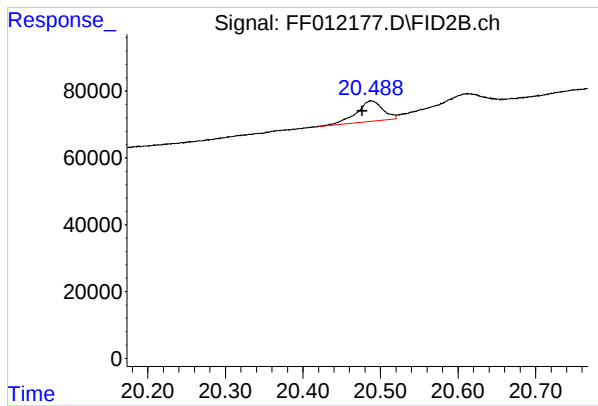

#16 N-HEXATRIACONTANE

R.T.: 20.488 min
Delta R.T.: 0.012 min
Response: 144065
Conc: 1.52 ug/ml

Instrument :
FID_F
ClientSampleId :