

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
 Data File : FF012189.D
 Signal(s) : FID2B.ch
 Acq On : 22 Feb 2023 16:52
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 23 00:50:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:12:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.040	1975526	16.651 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.937	105060	0.944 ug/ml
16) N-HEXATRIACONTANE	20.487	94111	0.992 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012189.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 16:52
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 00:50:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

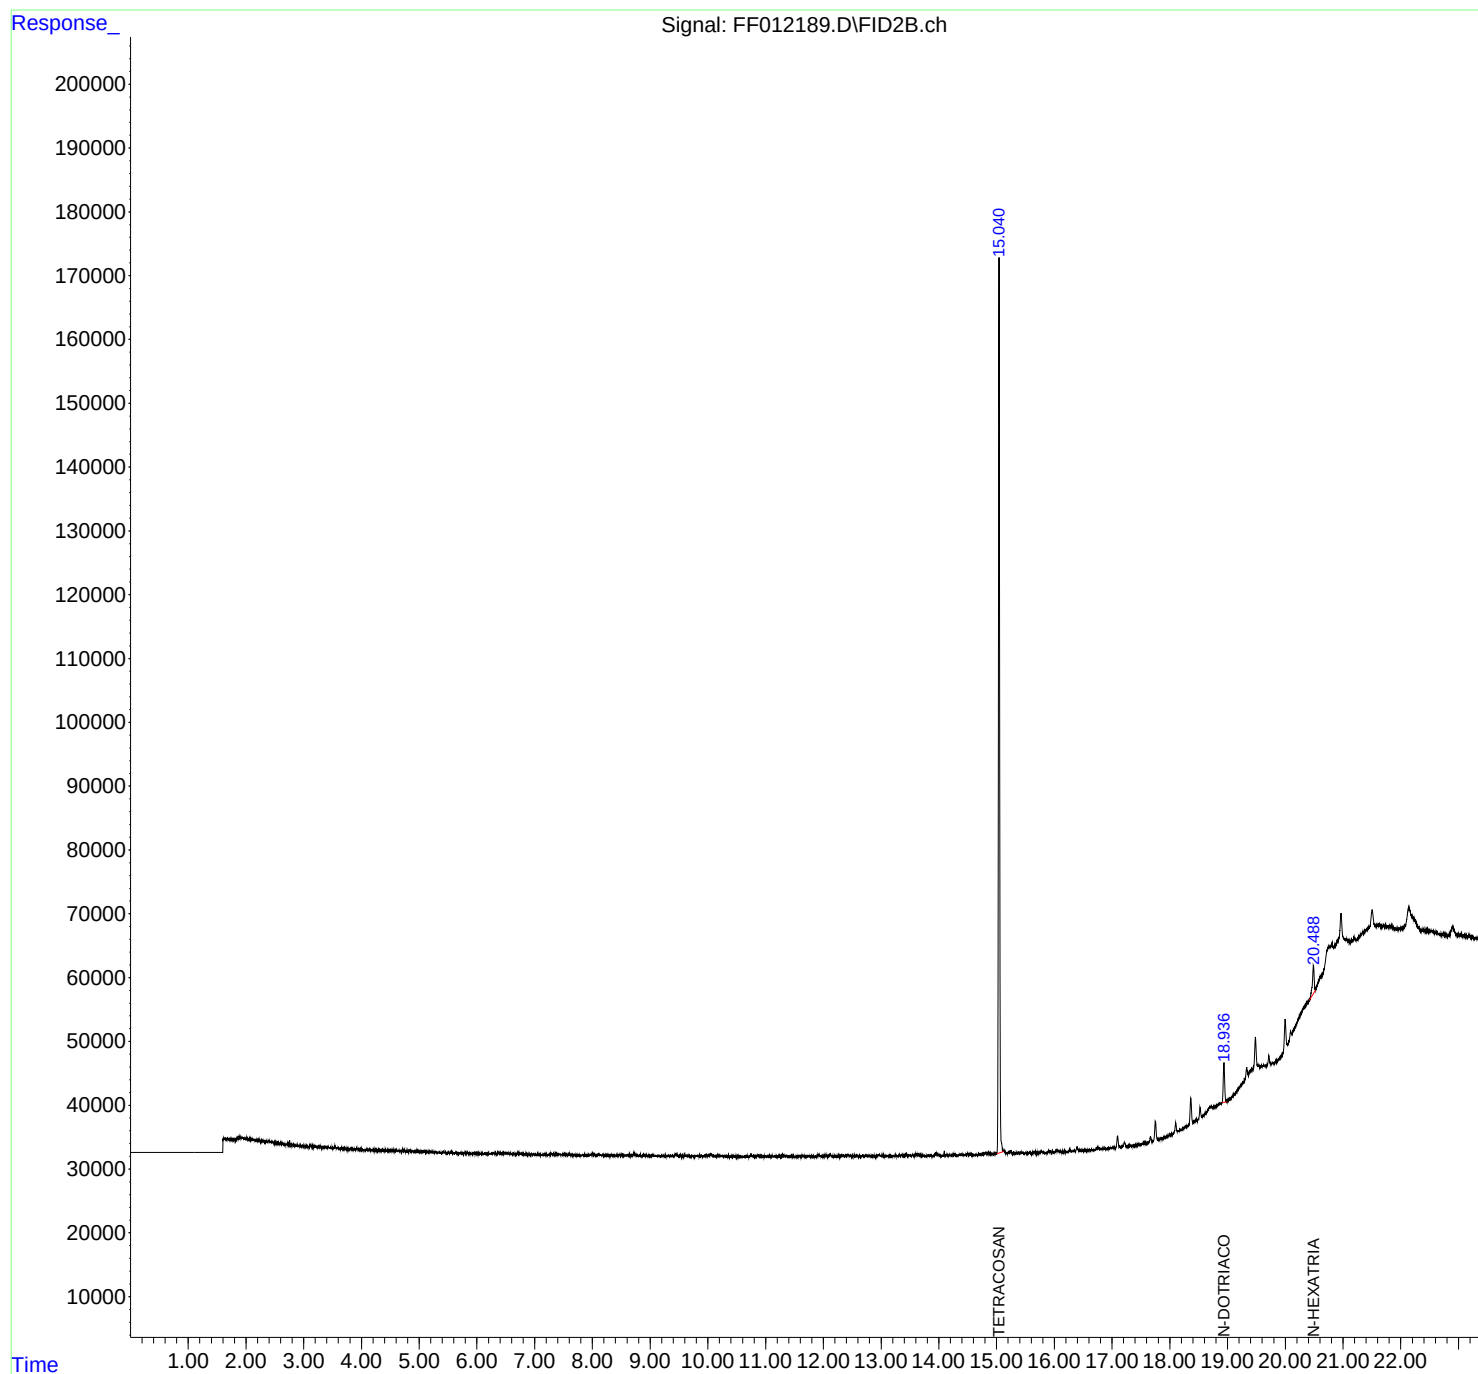

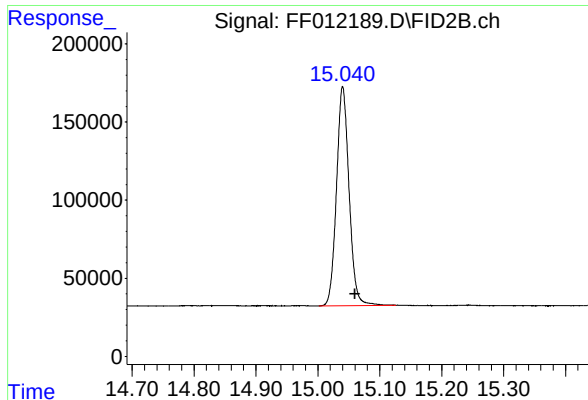


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.040 min
Delta R.T.: -0.020 min
Response: 1975526
Conc: 16.65 ug/ml

Instrument :


FID_F

ClientSampleId :

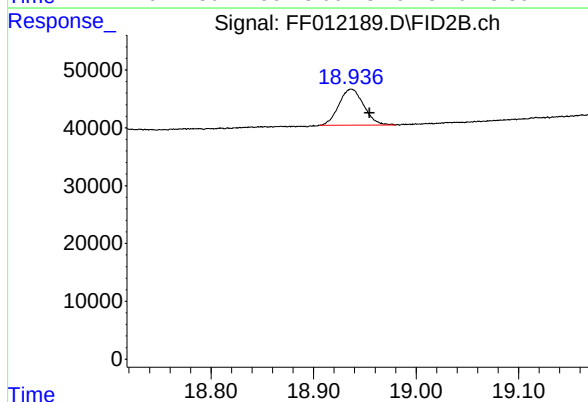

#14 N-DOTRIACONTANE

R.T.: 18.937 min
Delta R.T.: -0.018 min
Response: 105060
Conc: 0.94 ug/ml

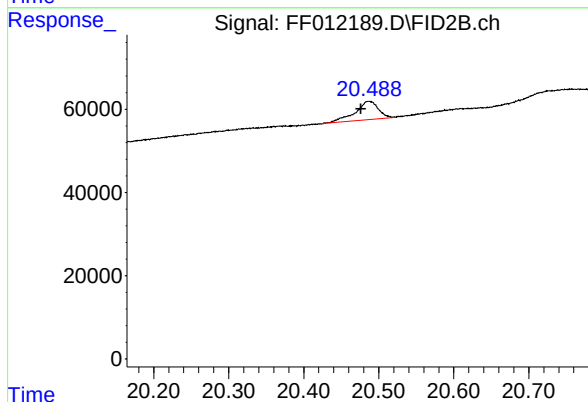

#16 N-HEXATRIACONTANE

R.T.: 20.487 min
Delta R.T.: 0.011 min
Response: 94111
Conc: 0.99 ug/ml