

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
 Data File : FF012193.D
 Signal(s) : FID2B.ch
 Acq On : 22 Feb 2023 19:20
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 23 00:51:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:12:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.759	2660311	19.581 ug/ml
12) N-OCTACOSANE	17.212	2604422	21.219 ug/ml
14) N-DOTRIACONTANE	18.935	247706	2.225 ug/ml
16) N-HEXATRIACONTANE	20.485	254899	2.688 ug/ml
18) N-TETRACONTANE	22.136	331114	3.636 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012193.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 19:20
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 00:51:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

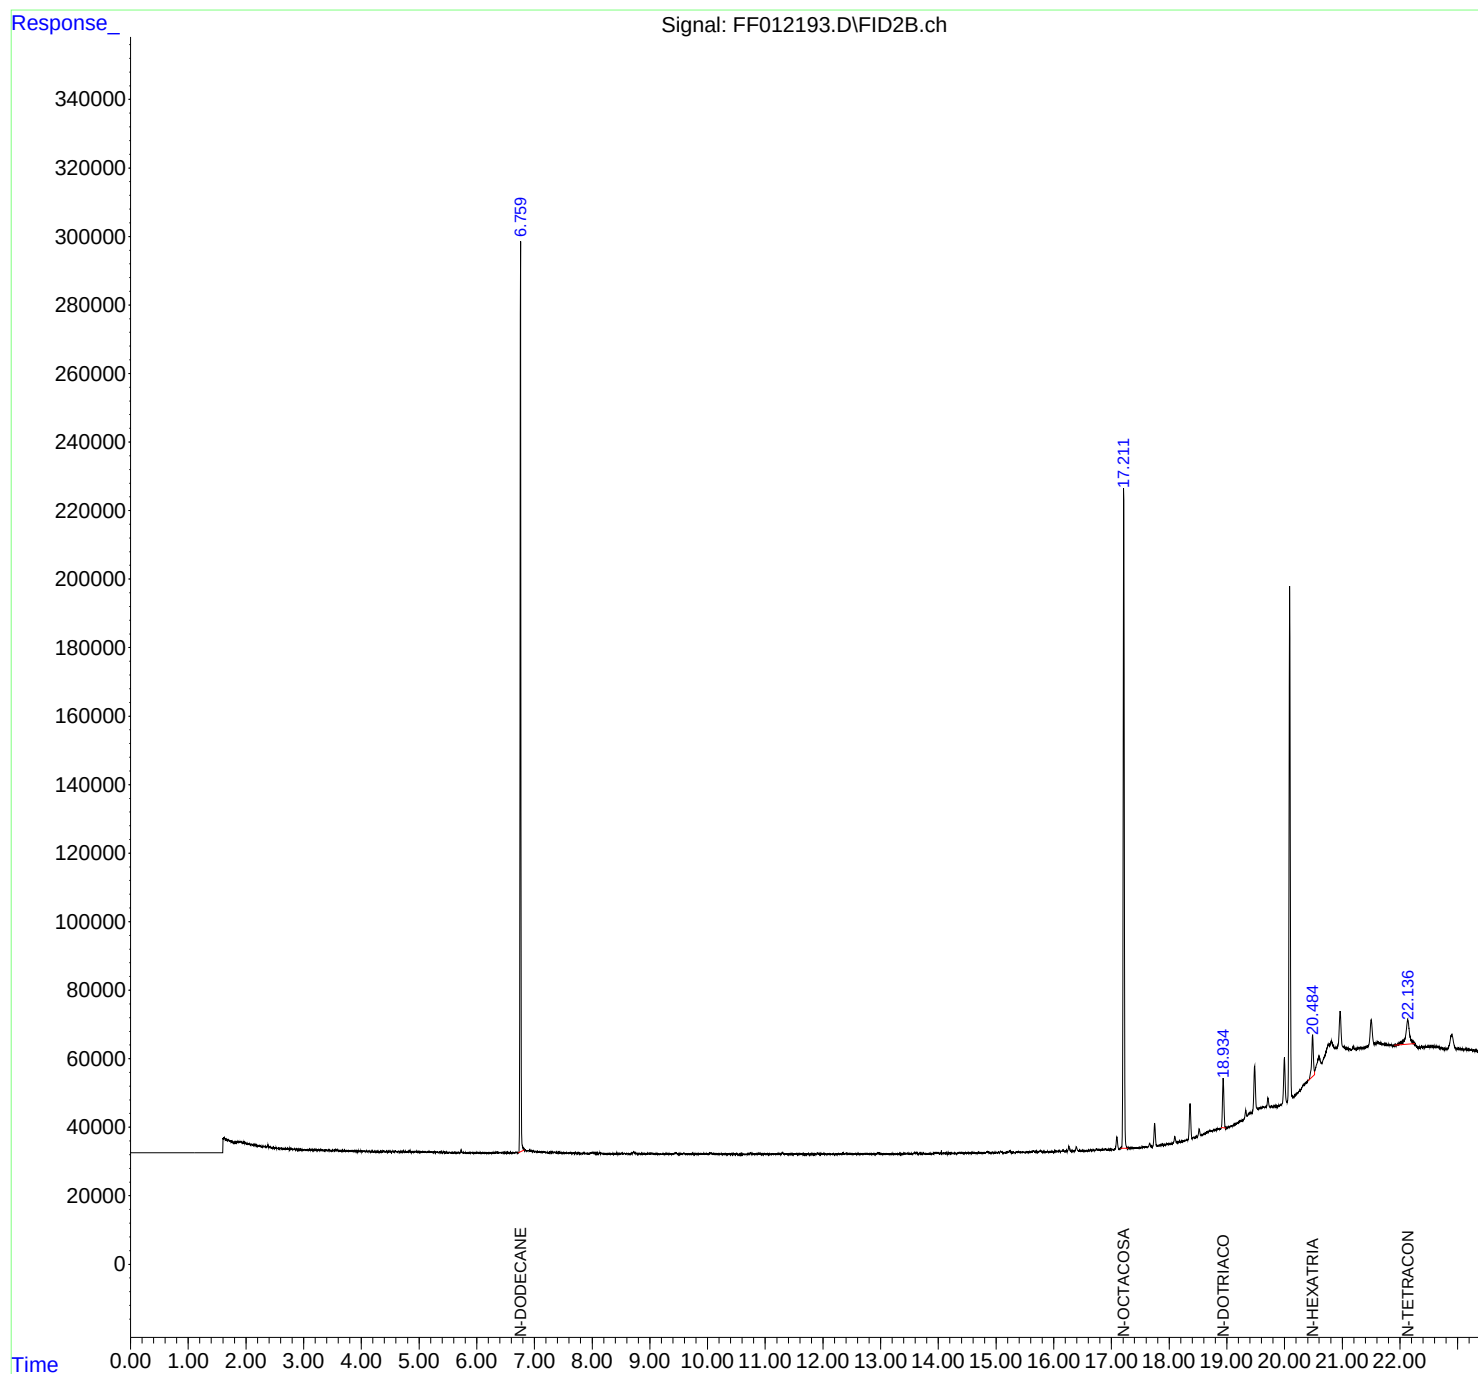

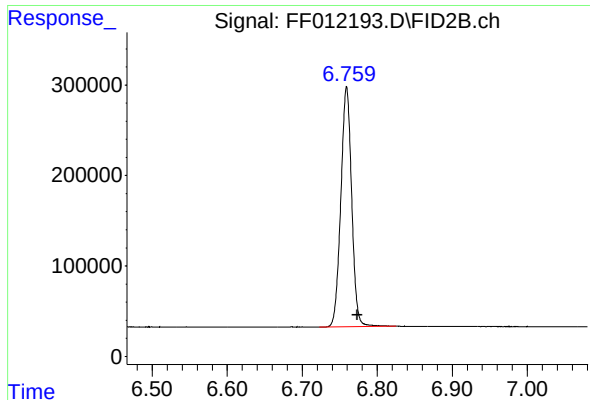


#3 N-DODECANE

R.T.: 6.759 min
Delta R.T.: -0.014 min
Response: 2660311
Conc: 19.58 ug/ml

Instrument :


FID_F

ClientSampleId :

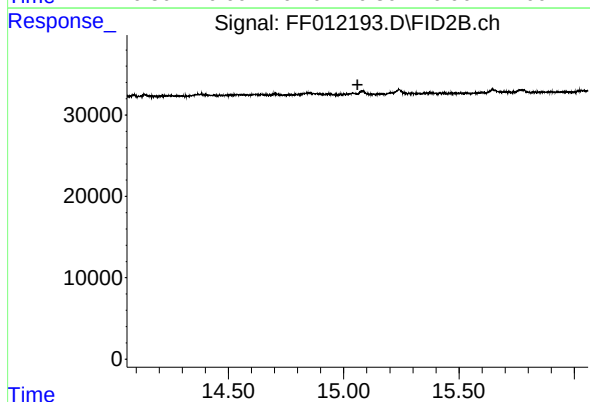


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.060 min
Response: 0
Conc: N.D.

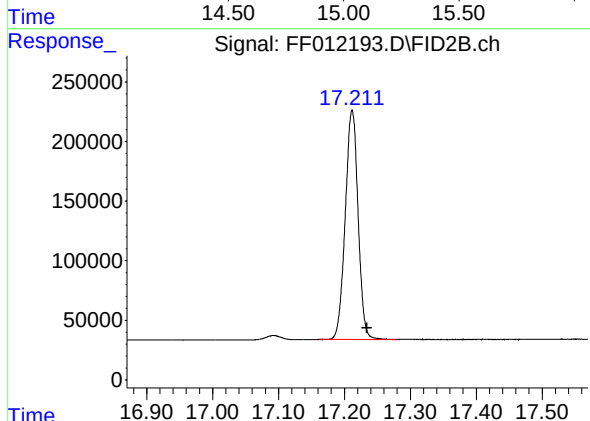


#12 N-OCTACOSANE

R.T.: 17.212 min
Delta R.T.: -0.023 min
Response: 2604422
Conc: 21.22 ug/ml

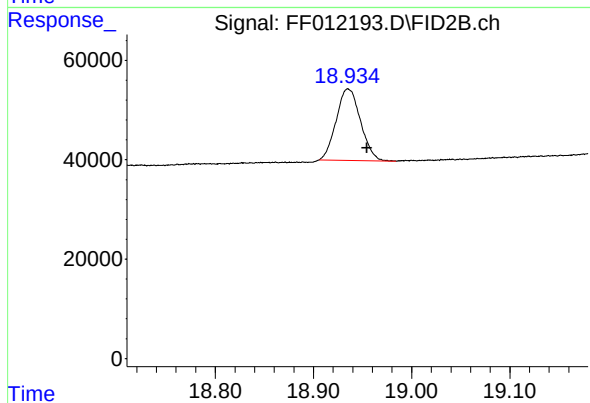

#14 N-DOTRIACONTANE


R.T.: 18.935 min
Delta R.T.: -0.019 min
Response: 247706
Conc: 2.22 ug/ml

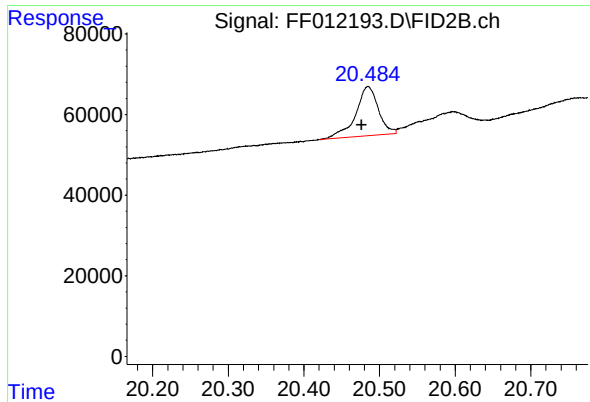

#16 N-HEXATRIACONTANE

R.T.: 20.485 min
Delta R.T.: 0.008 min
Response: 254899
Conc: 2.69 ug/ml

Instrument :
FID_F
ClientSampleId :

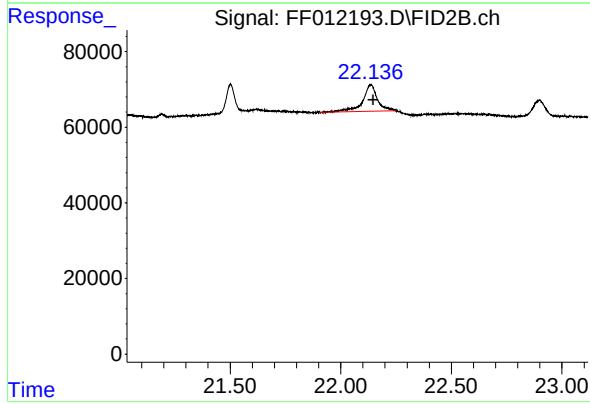

#18 N-TETRACONTANE

R.T.: 22.136 min
Delta R.T.: -0.011 min
Response: 331114
Conc: 3.64 ug/ml