

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012178.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 10:21
Operator : YP\AJ
Sample : PB150993BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB150993BL

Integration File: autoint1.e
Quant Time: Feb 23 00:49:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.043	2276213	19.186 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012178.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 10:21
Operator : YP\AJ
Sample : PB150993BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB150993BL

Integration File: autoint1.e
Quant Time: Feb 23 00:49:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

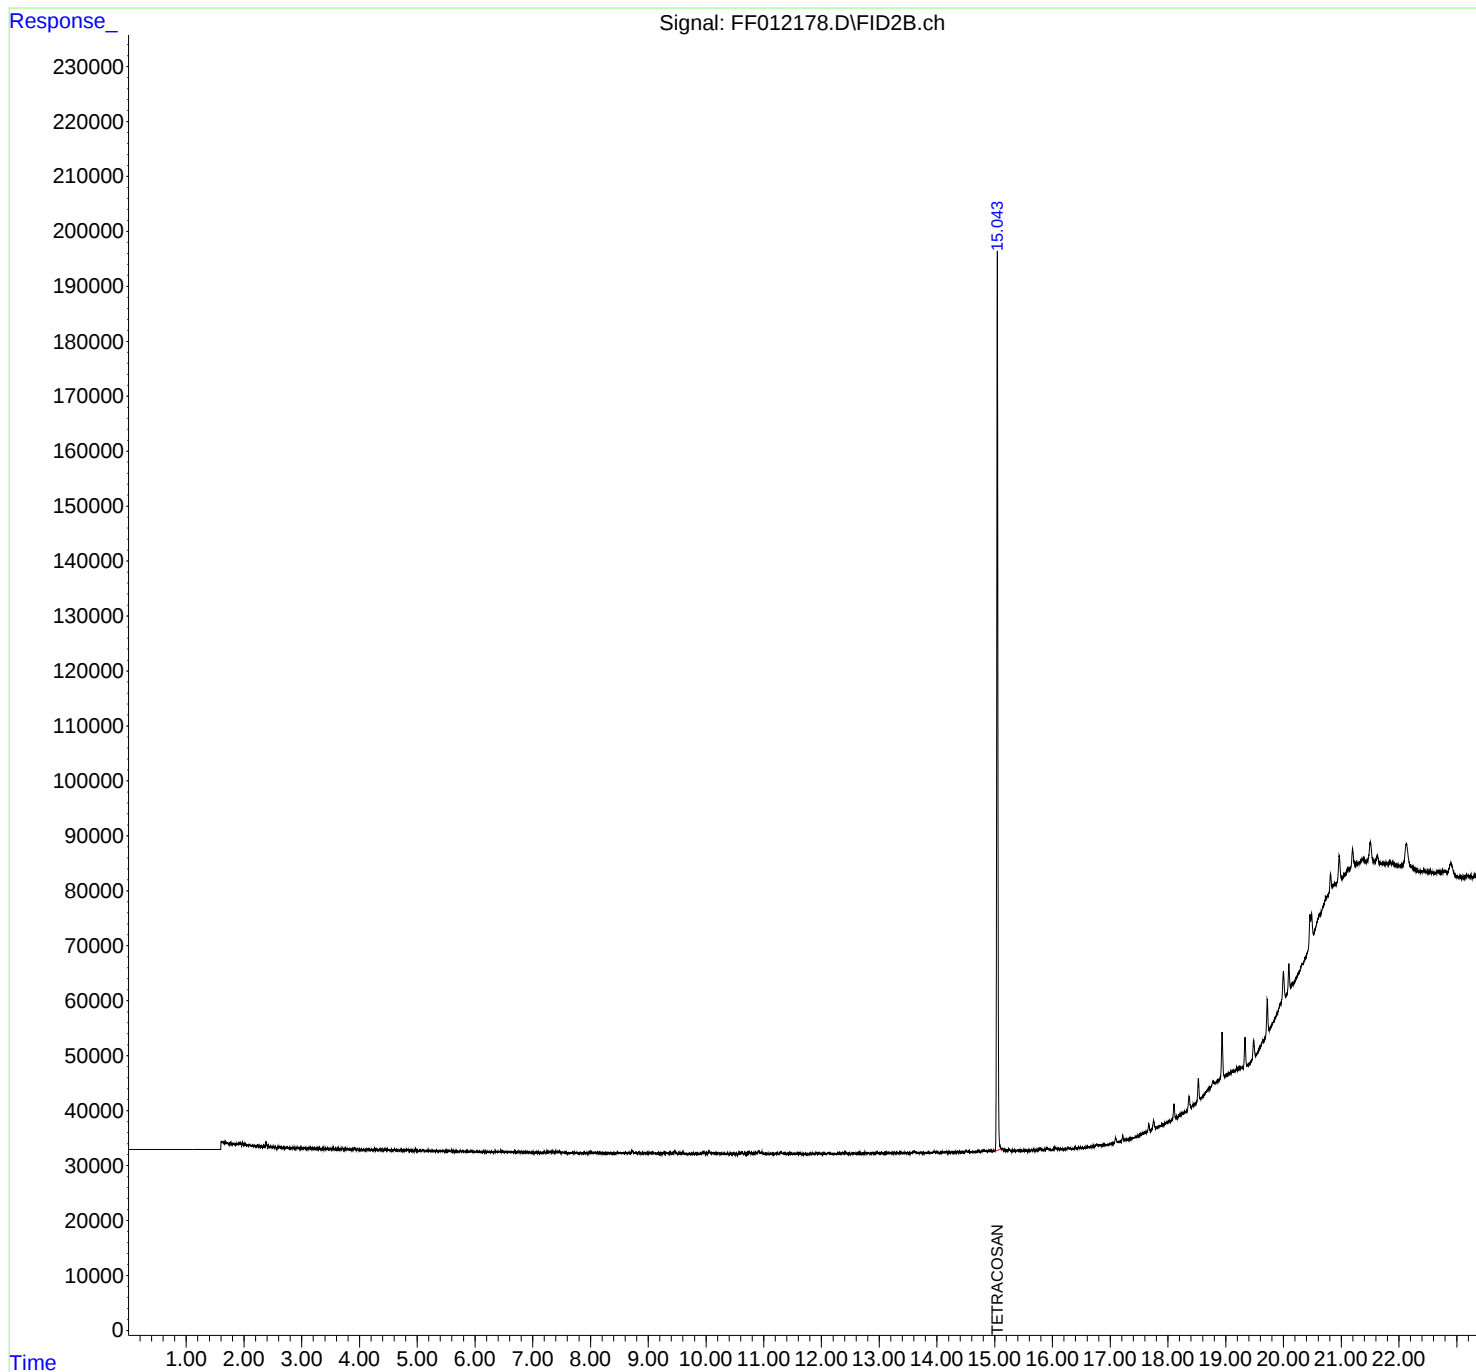

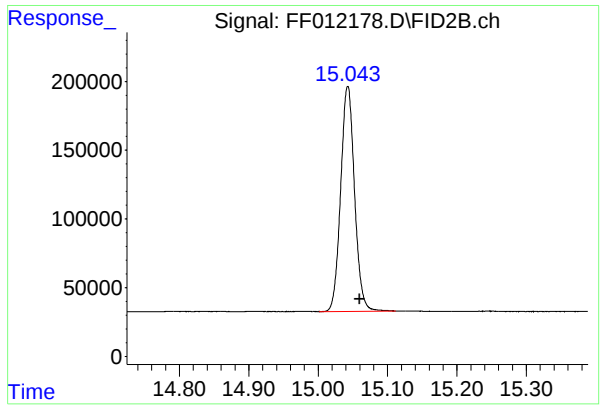

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.043 min
Delta R.T.: -0.017 min
Response: 2276213
Conc: 19.19 ug/ml

Instrument :
FID_F
ClientSampleId :
PB150993BL