

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
 Data File : FF012192.D
 Signal(s) : FID2B.ch
 Acq On : 22 Feb 2023 18:50
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Feb 23 00:51:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
 Quant Title :
 QLast Update : Tue Feb 21 16:12:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.040	5625278	47.414 ug/ml
Target Compounds			
2) N-DECANE	4.599	6485999	48.370 ug/ml
3) N-DODECANE	6.762	6612704	48.673 ug/ml
4) N-TETRADECANE	8.588	6664246	47.871 ug/ml
5) N-HEXADECANE	10.194	6764677	47.522 ug/ml
6) N-OCTADECANE	11.636	6756123	47.526 ug/ml
7) N-EICOSANE	12.945	6672972	47.297 ug/ml
8) N-DOCOSANE	14.142	6380664	47.302 ug/ml
10) N-TETRACOSANE	15.244	6279734	47.399 ug/ml
11) N-HEXACOSANE	16.265	6059791	47.505 ug/ml
12) N-OCTACOSANE	17.214	5843293	47.608 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012192.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 18:50
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Feb 23 00:51:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

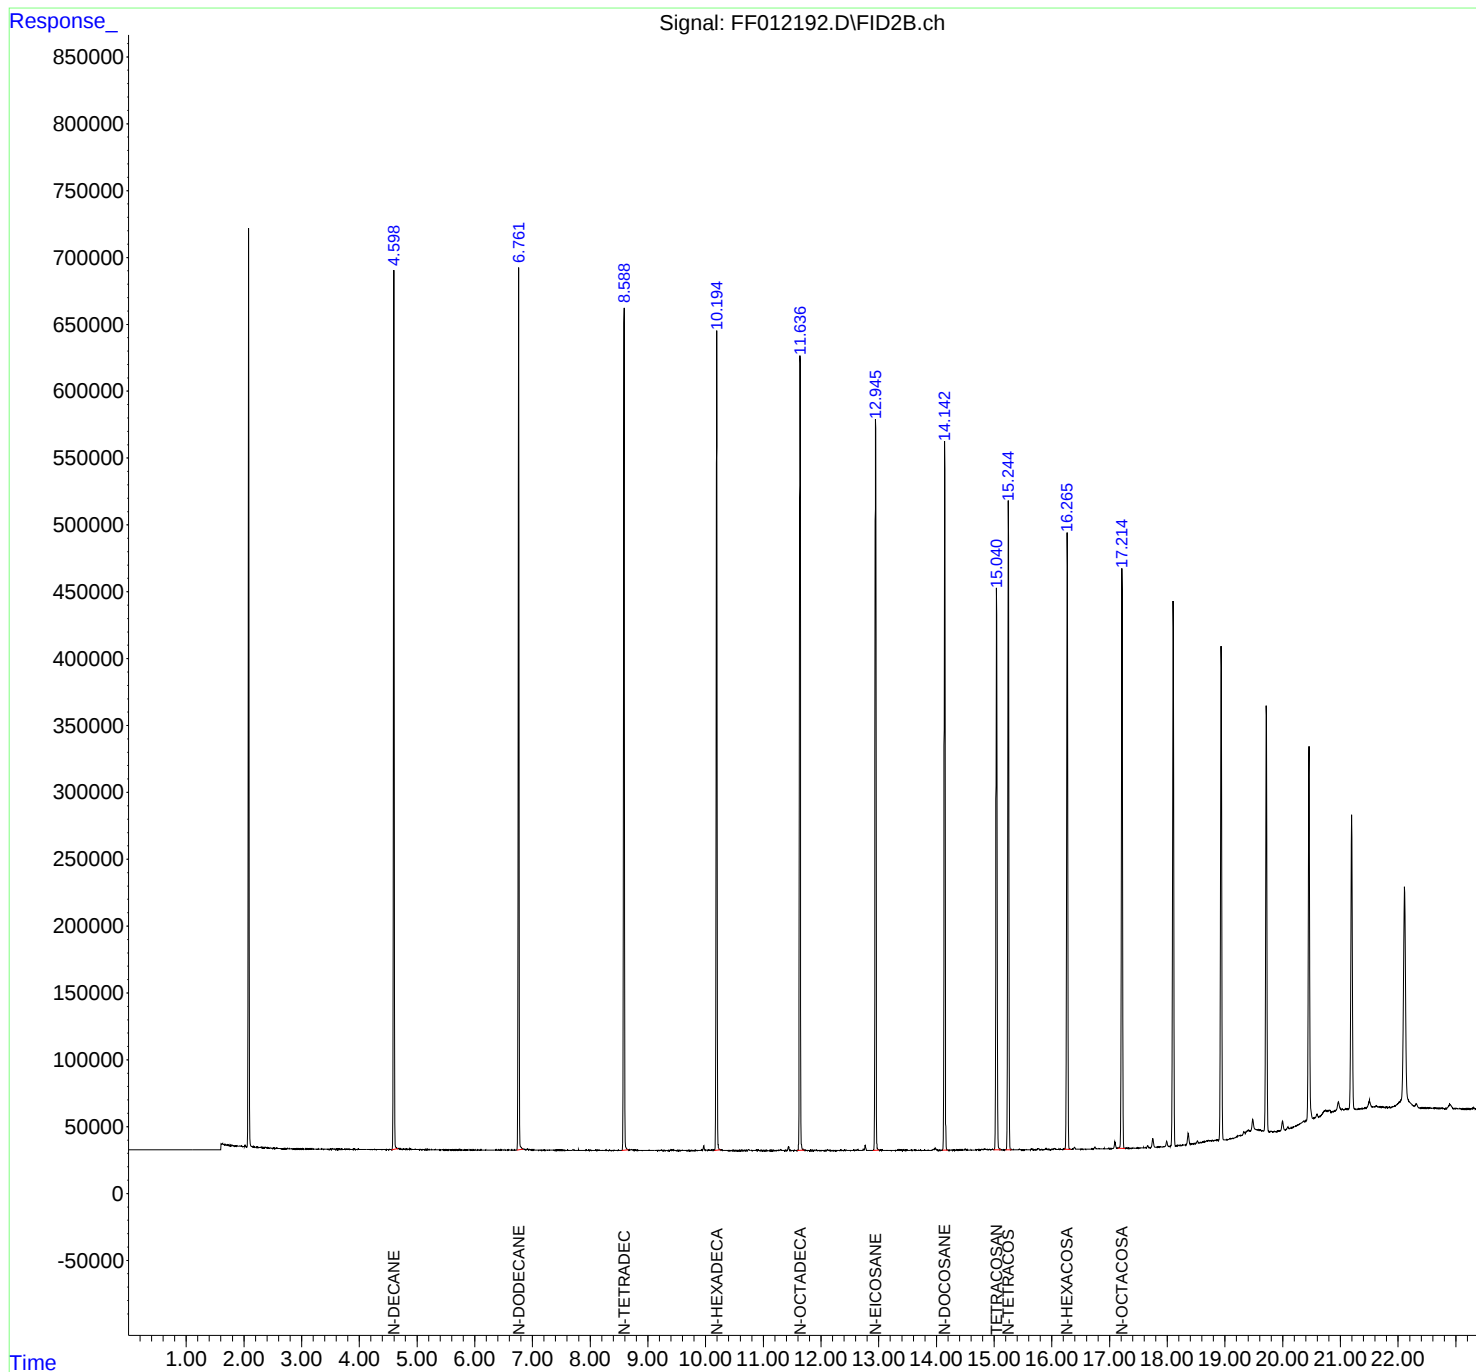


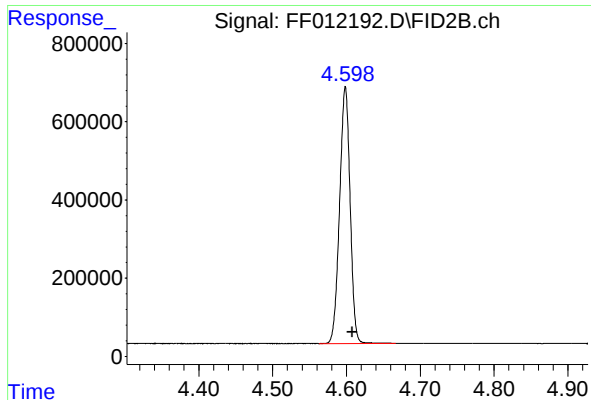

#2 N-DECANE


R.T.: 4.599 min
Delta R.T.: -0.010 min
Response: 6485999
Conc: 48.37 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

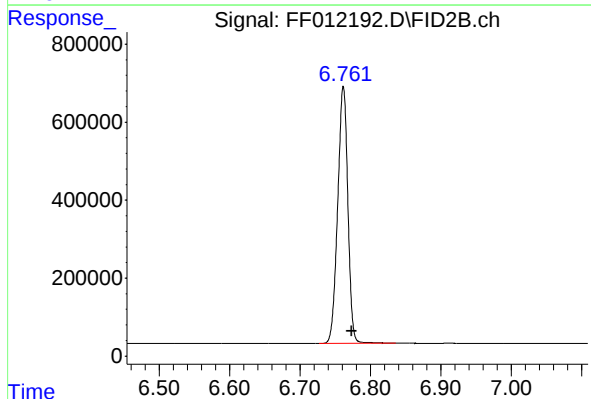


#3 N-DODECANE

R.T.: 6.762 min
Delta R.T.: -0.012 min
Response: 6612704
Conc: 48.67 ug/ml

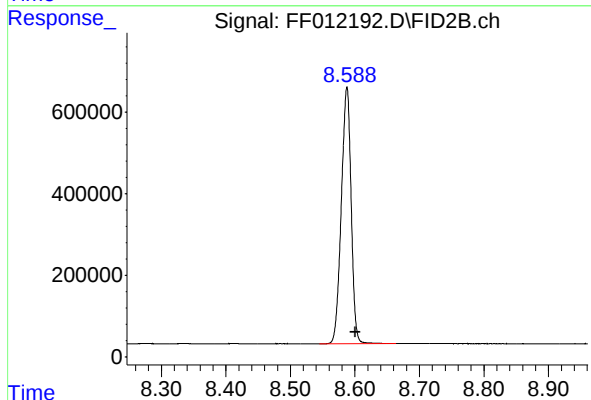


#4 N-TETRADECANE

R.T.: 8.588 min
Delta R.T.: -0.013 min
Response: 6664246
Conc: 47.87 ug/ml

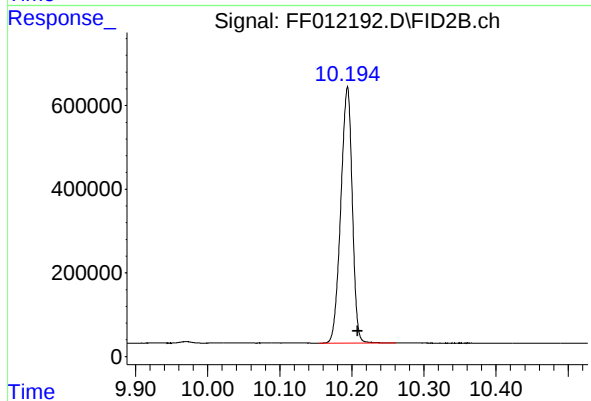

#5 N-HEXADECANE


R.T.: 10.194 min
Delta R.T.: -0.014 min
Response: 6764677
Conc: 47.52 ug/ml

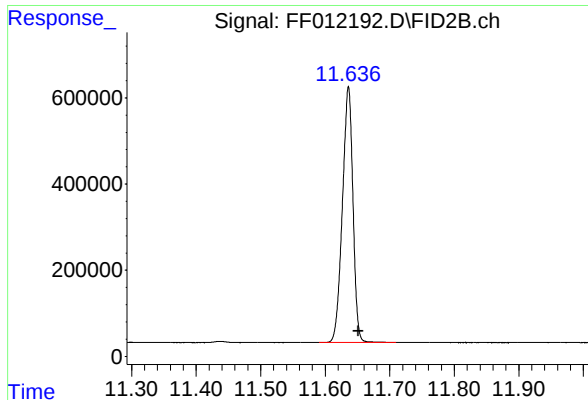

#6 N-OCTADECANE


R.T.: 11.636 min
Delta R.T.: -0.016 min
Response: 6756123
Conc: 47.53 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

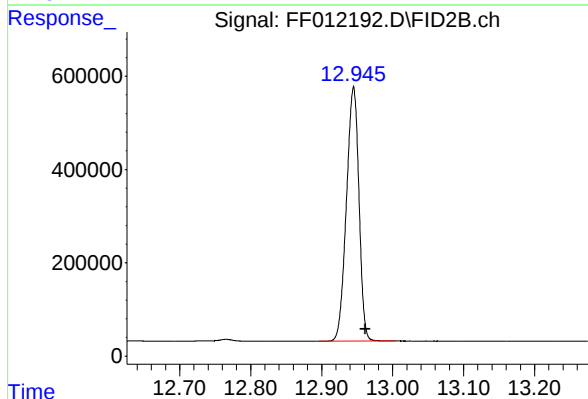


#7 N-EICOSANE

R.T.: 12.945 min
Delta R.T.: -0.016 min
Response: 6672972
Conc: 47.30 ug/ml

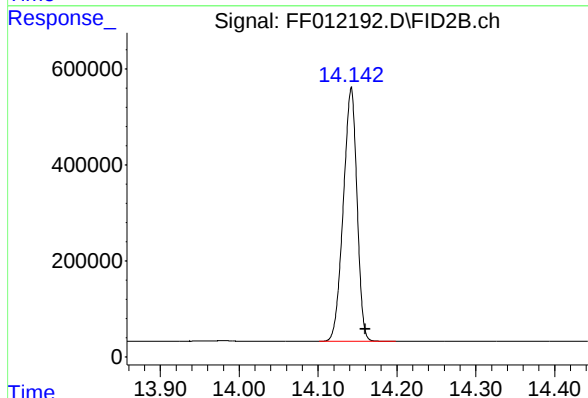


#8 N-DOCOSANE

R.T.: 14.142 min
Delta R.T.: -0.018 min
Response: 6380664
Conc: 47.30 ug/ml

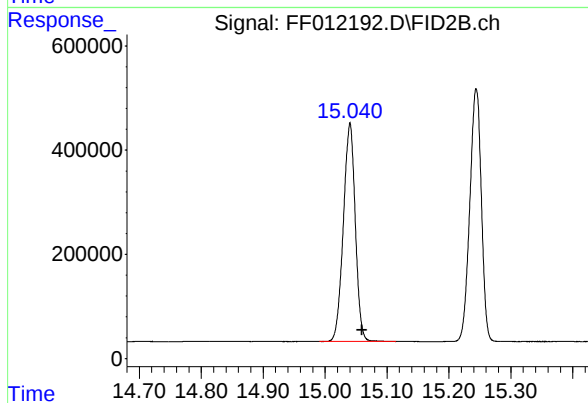

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.040 min
Delta R.T.: -0.019 min
Response: 5625278
Conc: 47.41 ug/ml

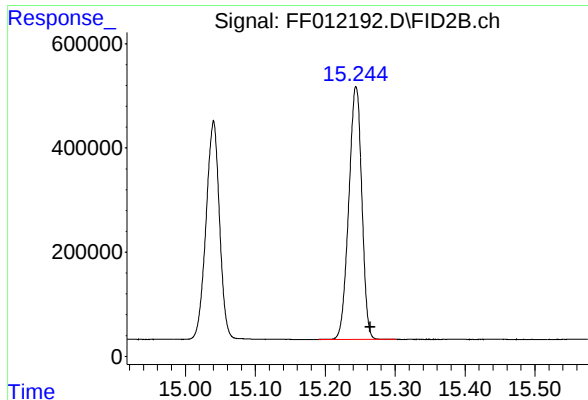

#10 N-TETRACOSANE


R.T.: 15.244 min
Delta R.T.: -0.020 min
Response: 6279734
Conc: 47.40 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

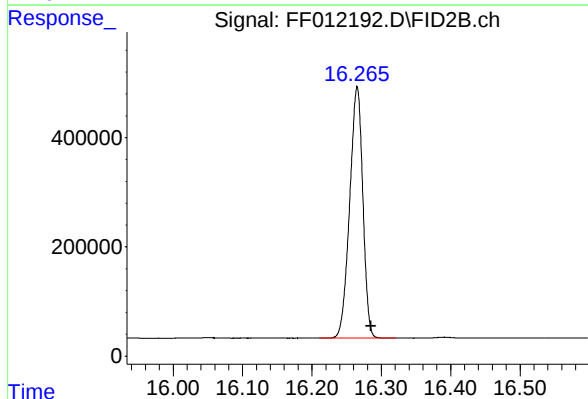

#11 N-HEXACOSANE

R.T.: 16.265 min
Delta R.T.: -0.020 min
Response: 6059791
Conc: 47.50 ug/ml

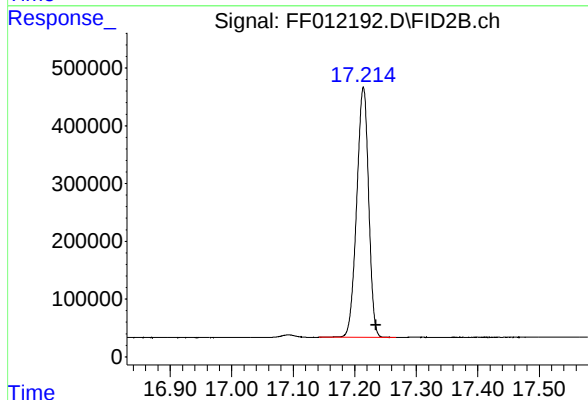

#12 N-OCTACOSANE

R.T.: 17.214 min
Delta R.T.: -0.020 min
Response: 5843293
Conc: 47.61 ug/ml