

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012194.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 19:49
Operator : YP\AJ
Sample : PB150992BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB150992BL

Integration File: autoint1.e
Quant Time: Feb 23 00:51:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.038	2032610	17.132 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012194.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 19:49
Operator : YP\AJ
Sample : PB150992BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB150992BL

Integration File: autoint1.e
Quant Time: Feb 23 00:51:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

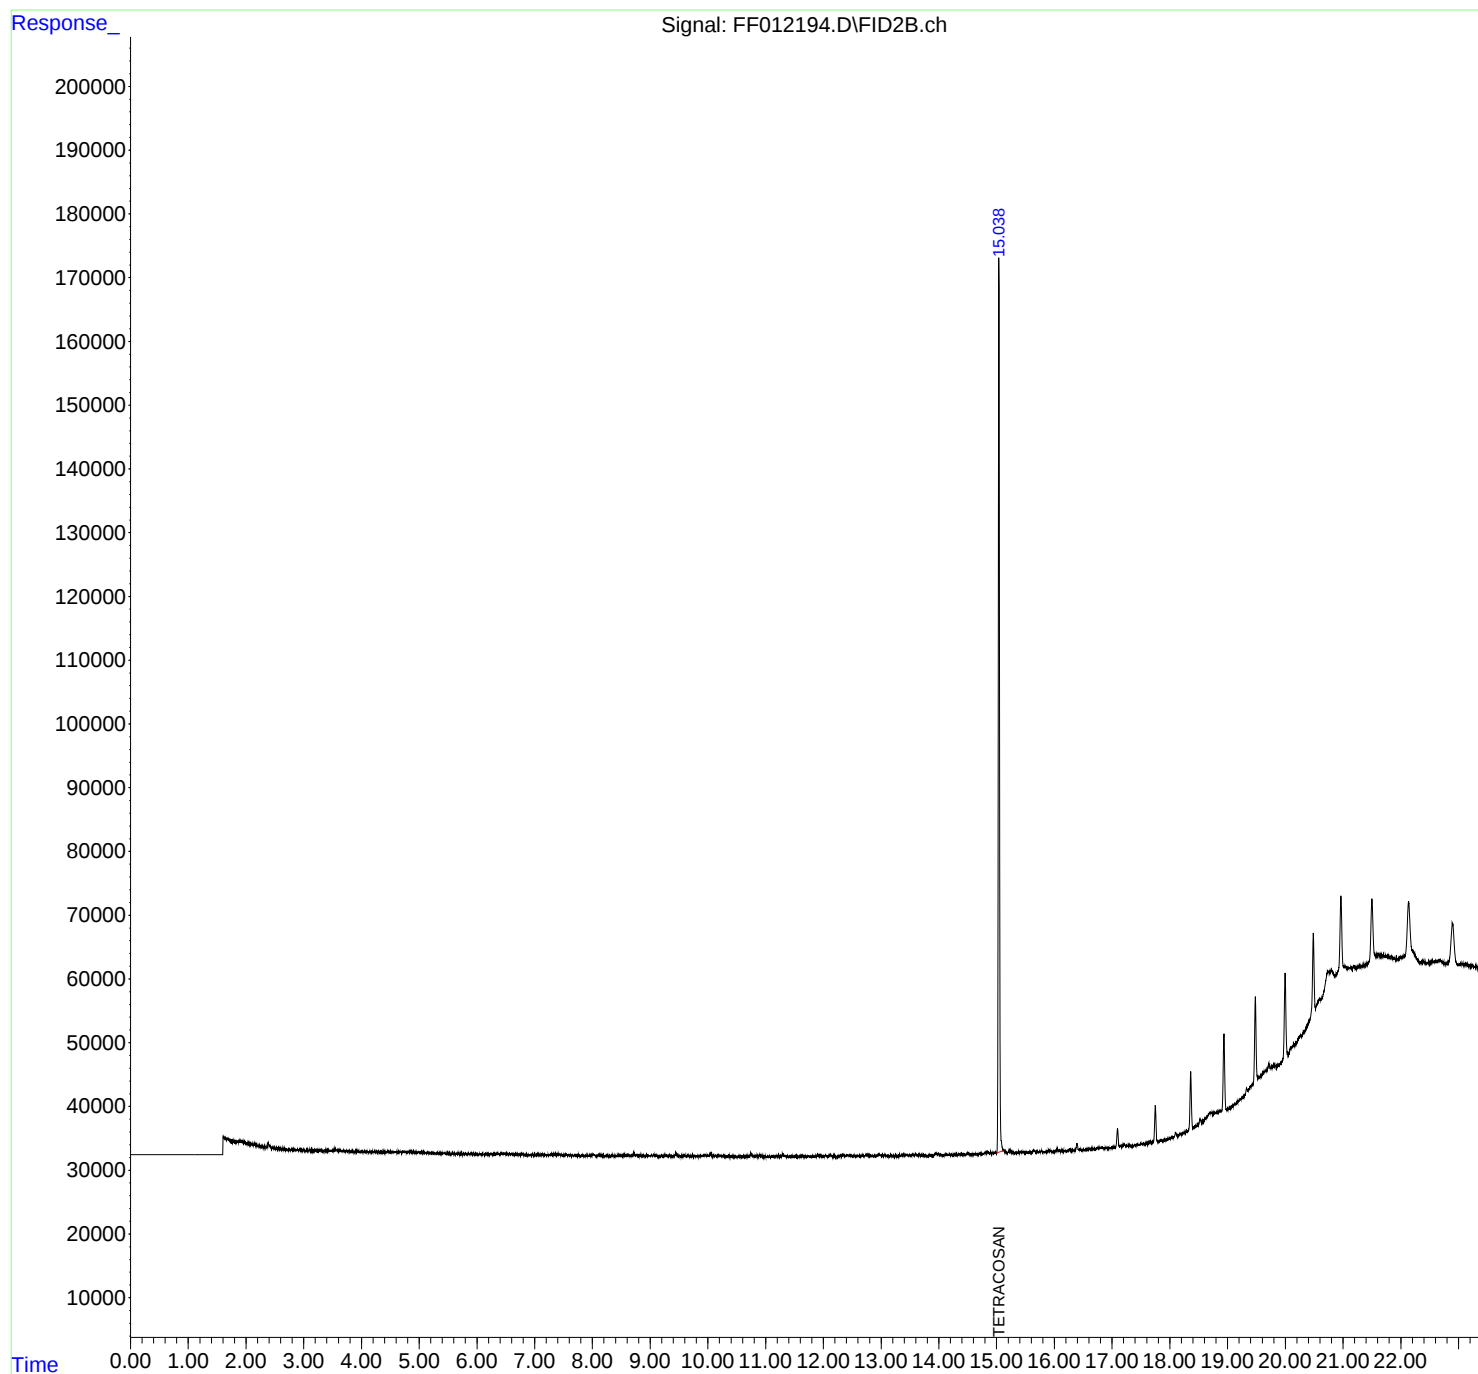

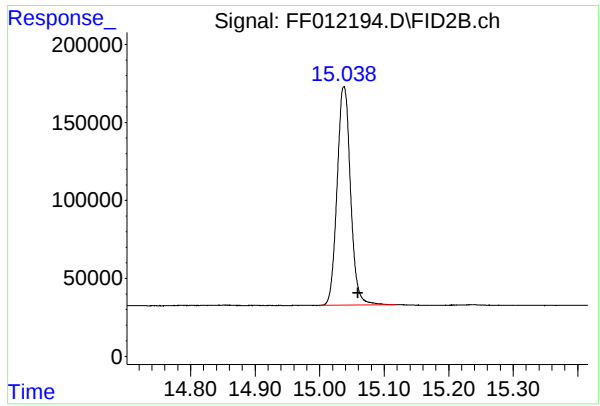

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.038 min
Delta R.T.: -0.022 min
Response: 2032610
Conc: 17.13 ug/ml

Instrument :
FID_F
ClientSampleId :
PB150992BL