

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012195.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 20:19
Operator : YP\AJ
Sample : PB150994BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB150994BL

Integration File: autoint1.e
Quant Time: Feb 23 00:51:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.037	2184420	18.412 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022223\
Data File : FF012195.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2023 20:19
Operator : YP\AJ
Sample : PB150994BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB150994BL

Integration File: autoint1.e
Quant Time: Feb 23 00:51:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

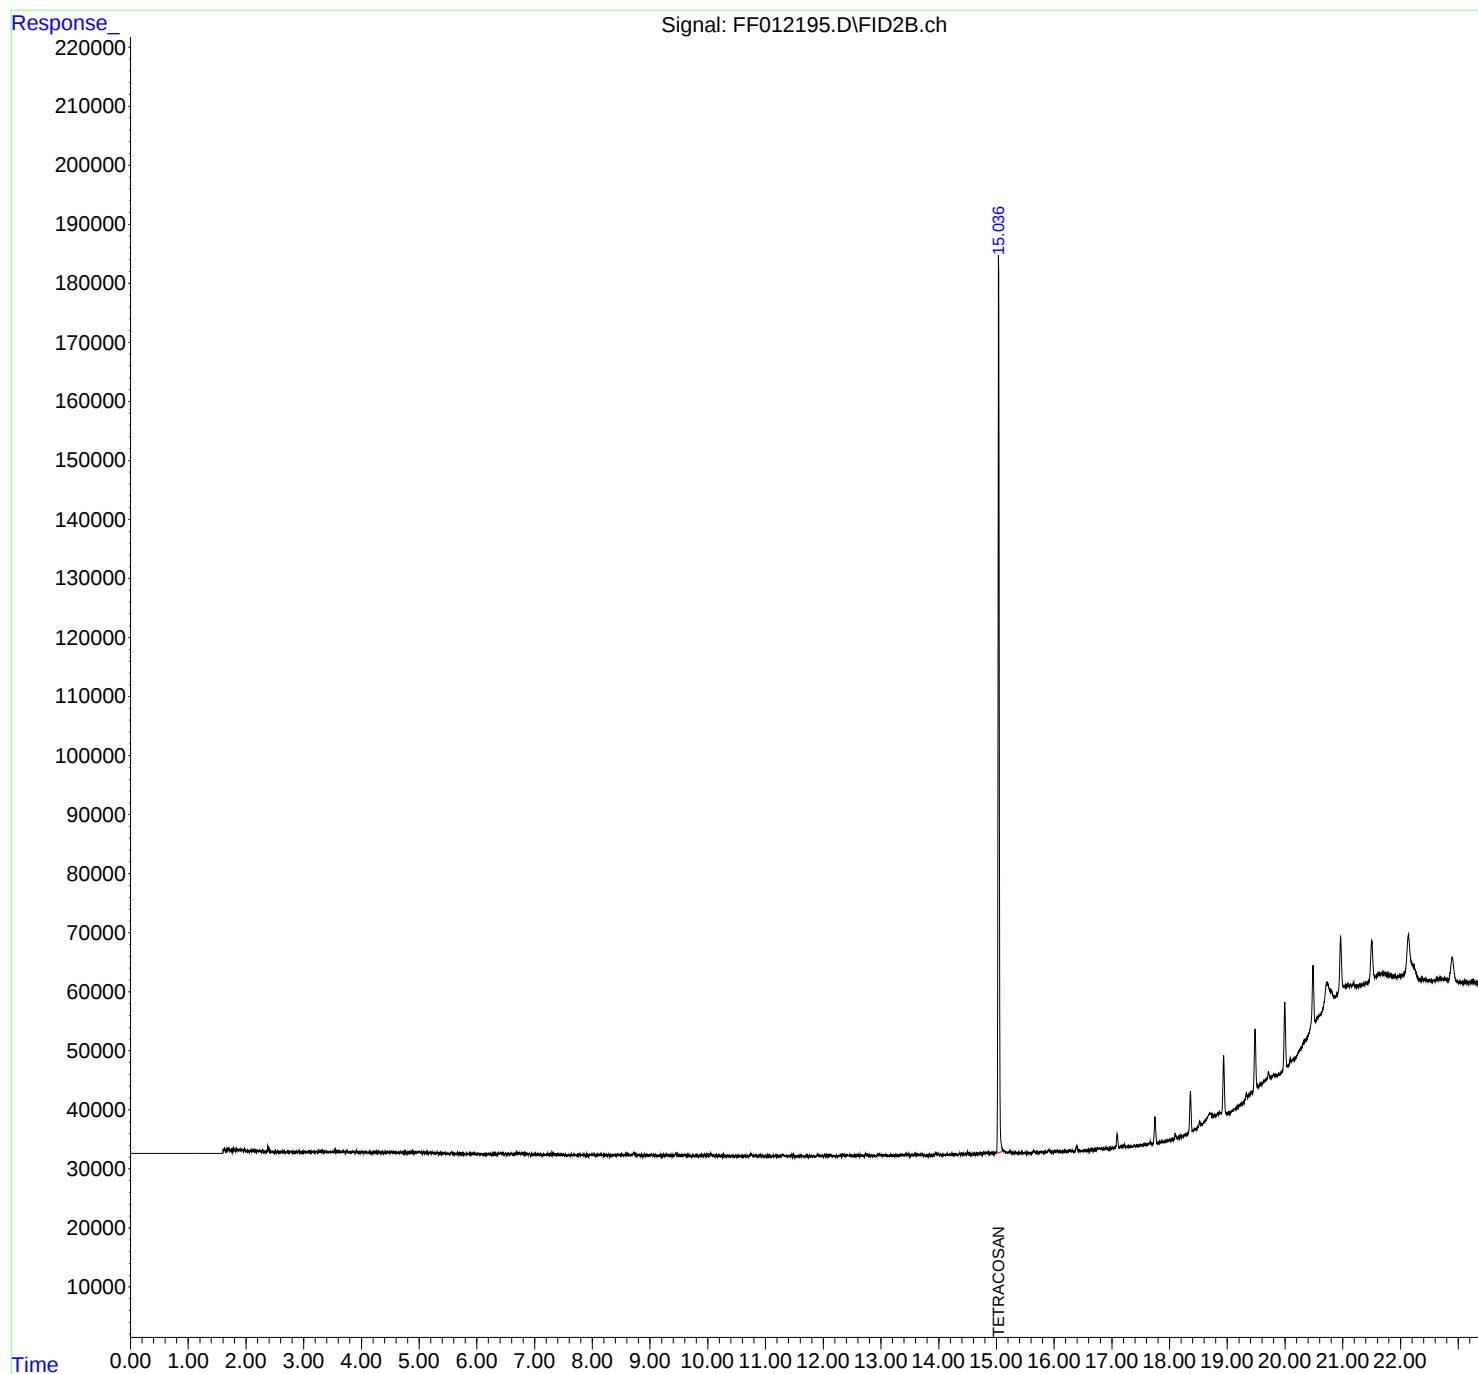

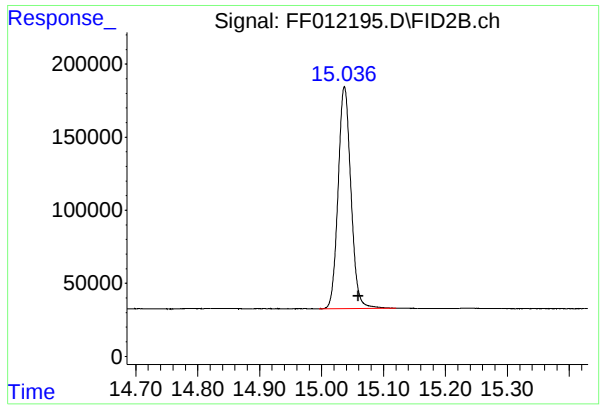

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.037 min

Delta R.T.: -0.023 min

Response: 2184420

Conc: 18.41 ug/ml

Instrument :

FID_F

ClientSampleId :

PB150994BL