

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022323\
Data File : FF012208.D
Signal(s) : FID2B.ch
Acq On : 23 Feb 2023 10:32
Operator : YP\AJ
Sample : PB151006BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 23 16:02:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.035	2451908	20.666 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.096	52694	0.451 ug/ml
14) N-DOTRIACONTANE	18.931	100526	0.903 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022323\
Data File : FF012208.D
Signal(s) : FID2B.ch
Acq On : 23 Feb 2023 10:32
Operator : YP\AJ
Sample : PB151006BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 23 16:02:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF022123.M
Quant Title :
QLast Update : Tue Feb 21 16:12:39 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

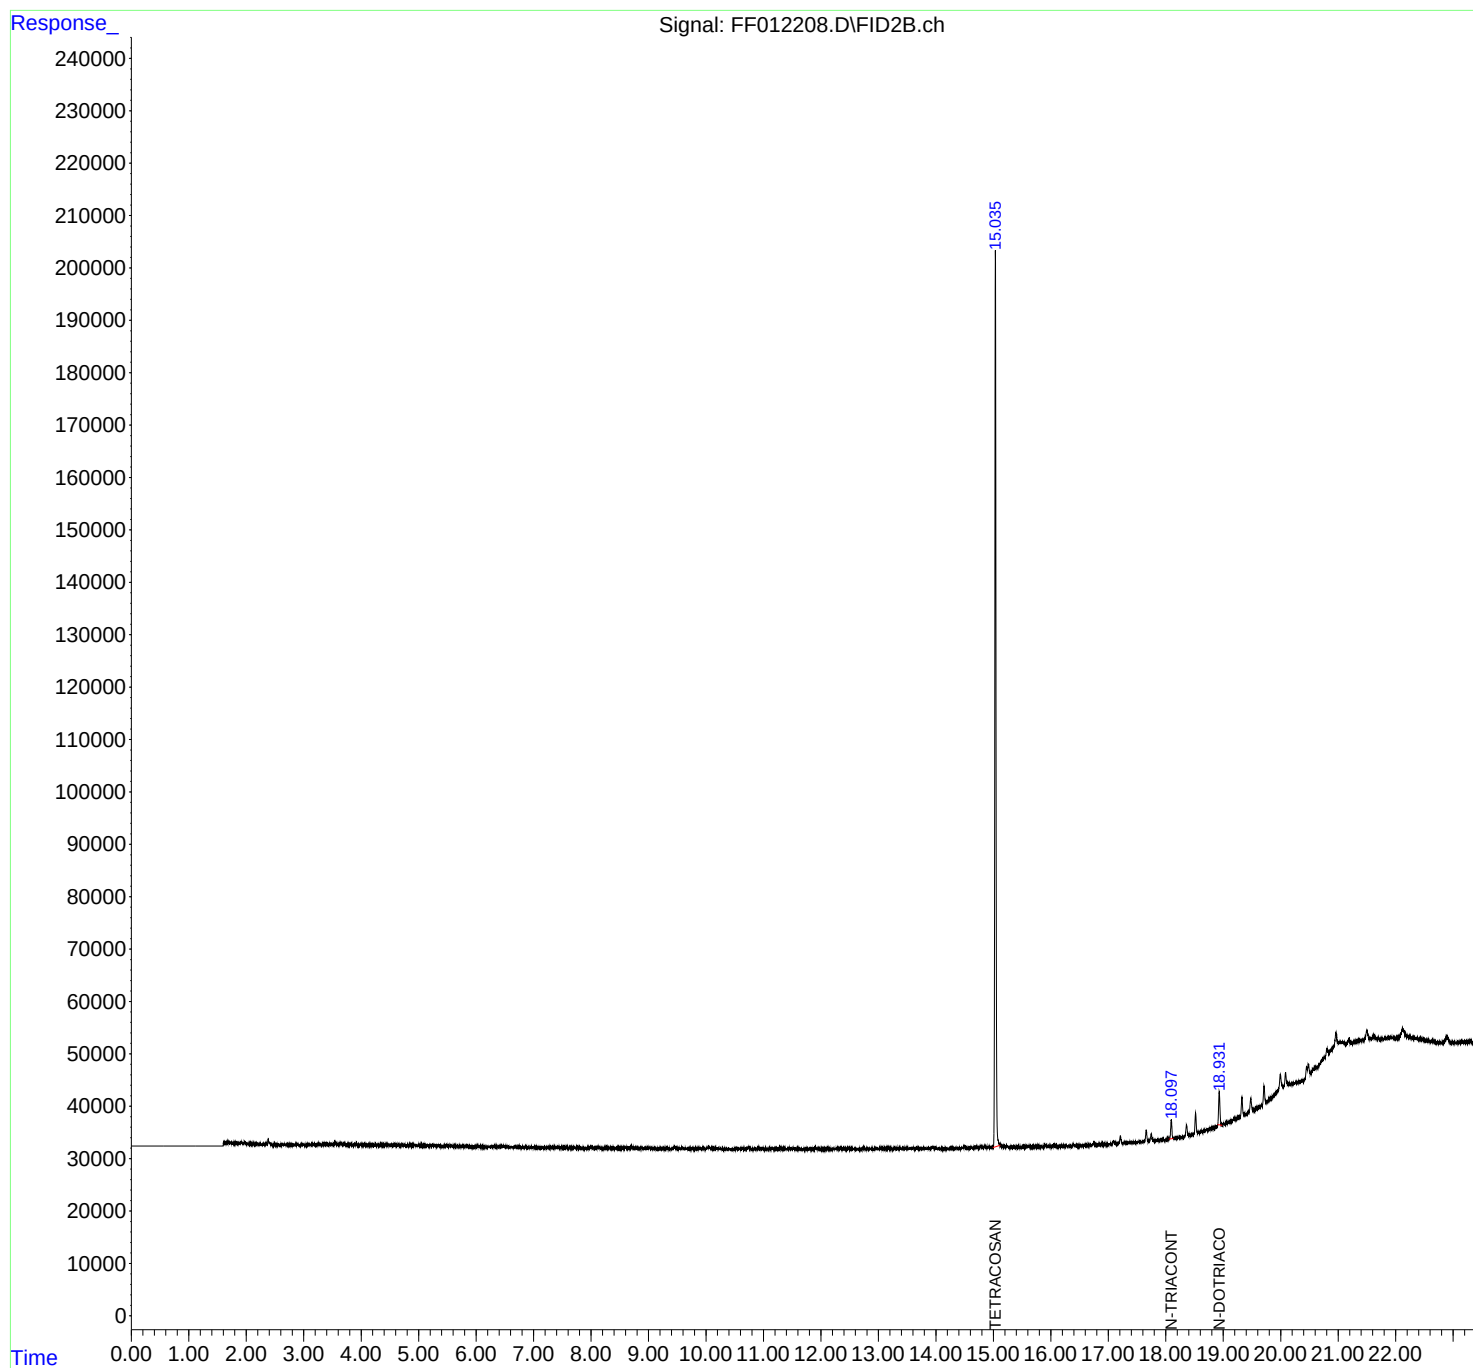

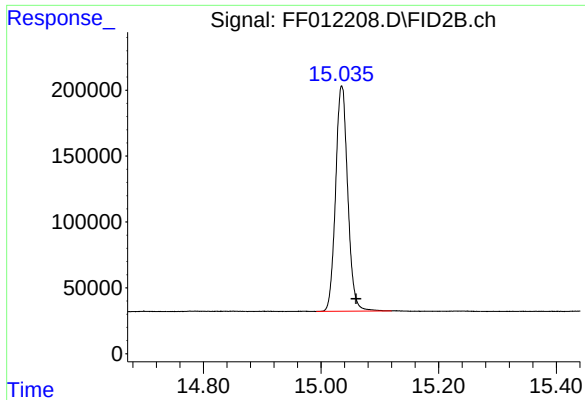


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.035 min
Delta R.T.: -0.024 min
Response: 2451908
Conc: 20.67 ug/ml

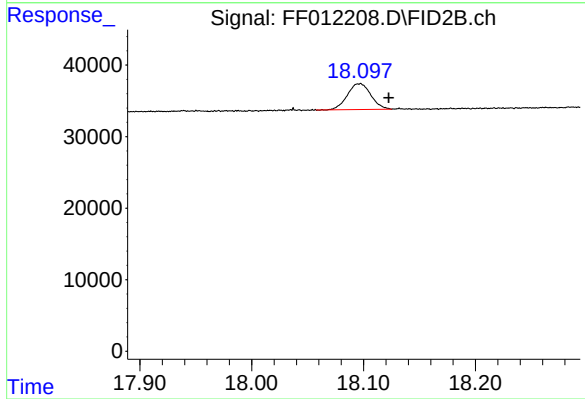

#13 N-TRIACONTANE

R.T.: 18.096 min
Delta R.T.: -0.026 min
Response: 52694
Conc: 0.45 ug/ml

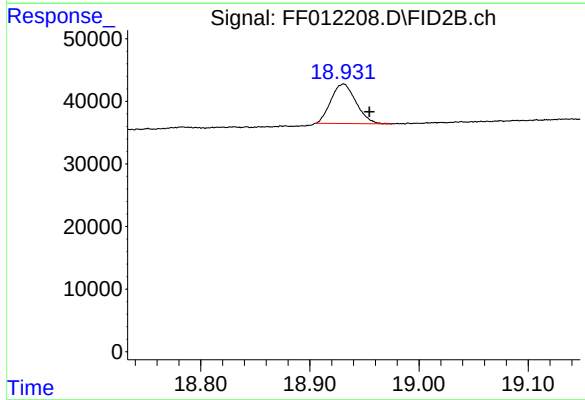

#14 N-DOTRIACONTANE

R.T.: 18.931 min
Delta R.T.: -0.024 min
Response: 100526
Conc: 0.90 ug/ml