

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
 Data File : FF006460.D
 Signal(s) : FID2B.ch
 Acq On : 24 Feb 2020 12:03
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 25 00:29:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.377	3802804	27.824 ug/ml
10) N-TETRACOSANE	14.785	239718	1.716 ug/ml
12) N-OCTACOSANE	16.769	3588307	26.001 ug/ml
13) N-TRIACONTANE	17.652	279149	2.019 ug/ml
14) N-DOTRIACONTANE	18.482	299512	2.277 ug/ml
15) N-TETRATRIACONTANE	19.264	206848	1.842 ug/ml
16) N-HEXATRIACONTANE	20.002	228217	2.358 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
Data File : FF006460.D
Signal(s) : FID2B.ch
Acq On : 24 Feb 2020 12:03
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 25 00:29:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

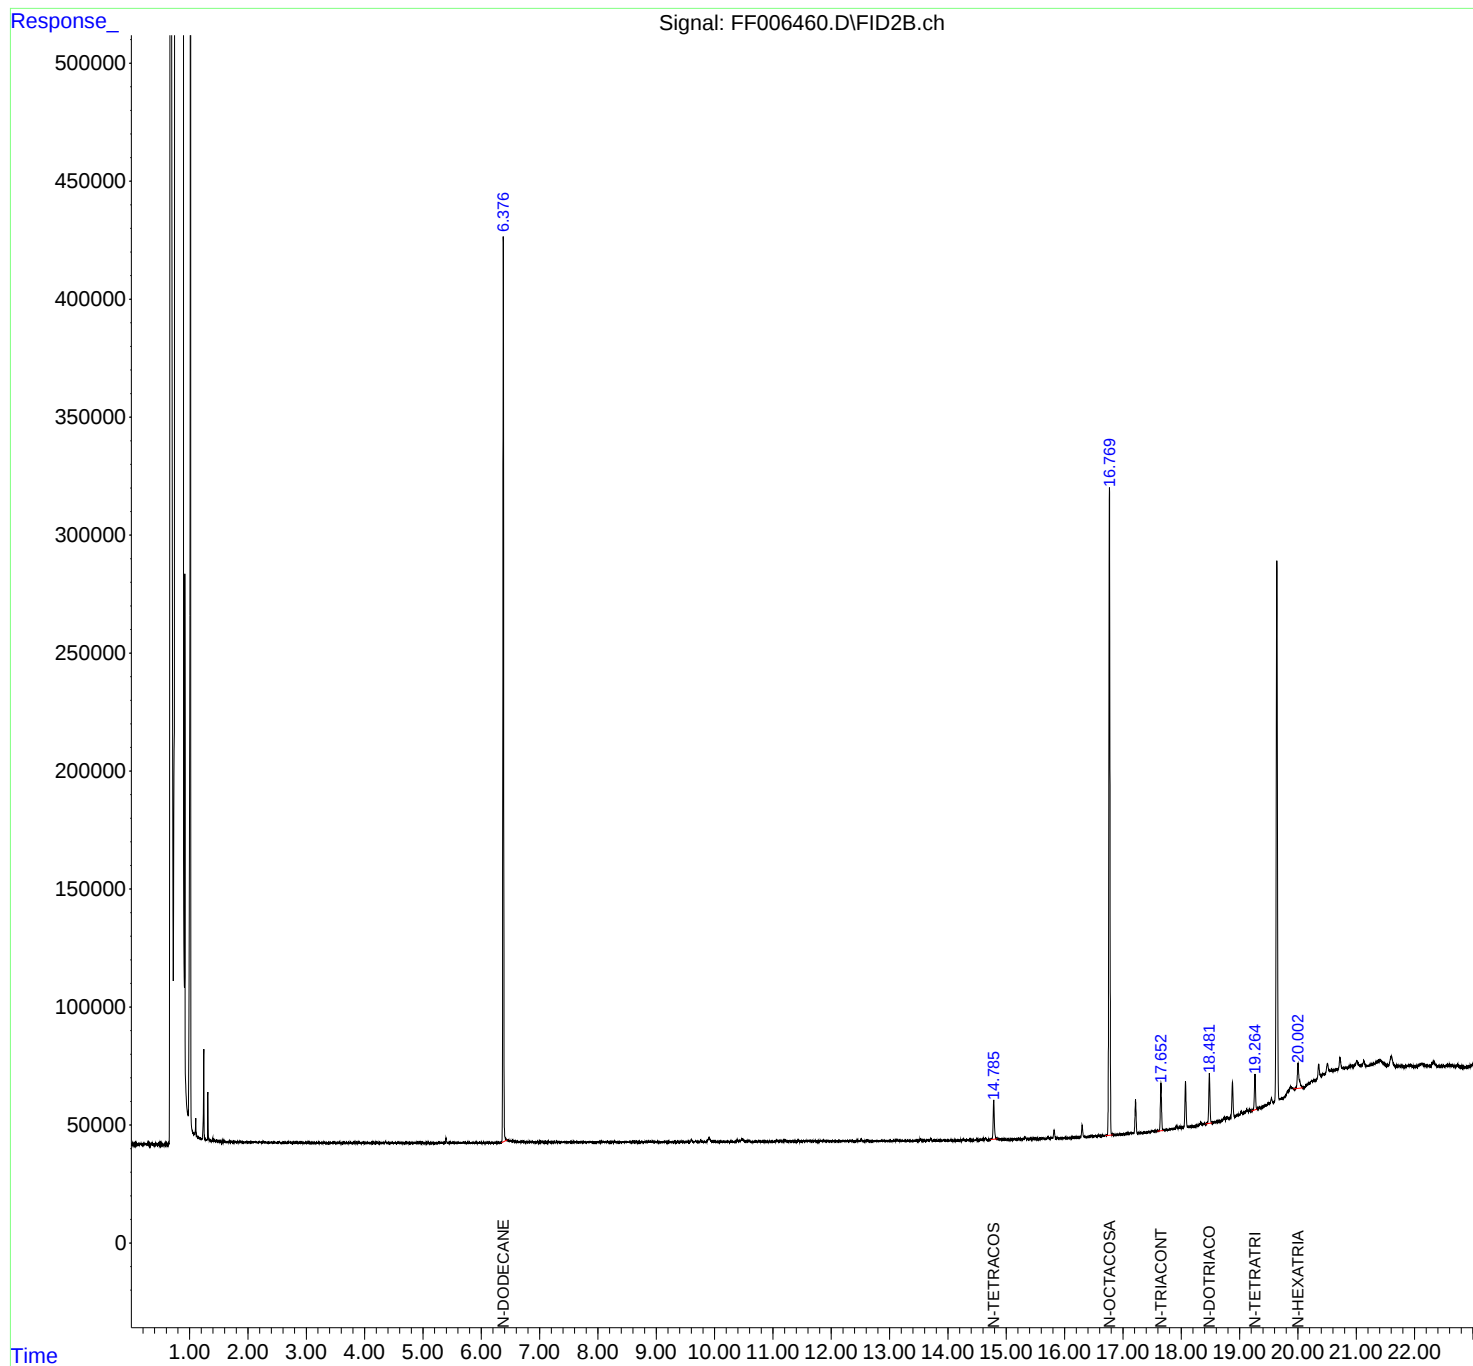


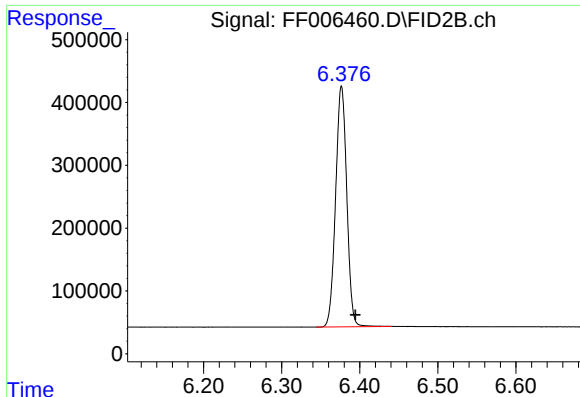

#3 N-DODECANE


R.T.: 6.377 min
Delta R.T.: -0.018 min
Response: 3802804
Conc: 27.82 ug/ml

Instrument :
FID_F
ClientSampleId :

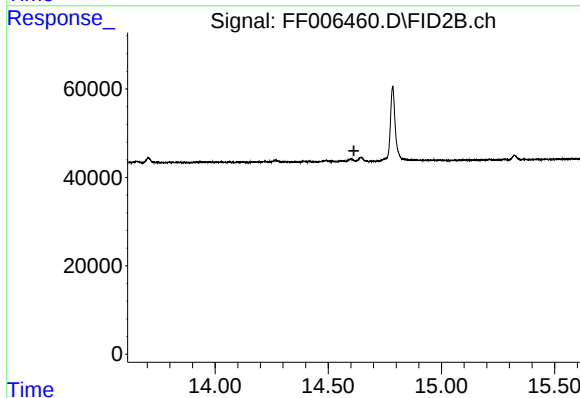


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.613 min
Response: 0
Conc: N.D.

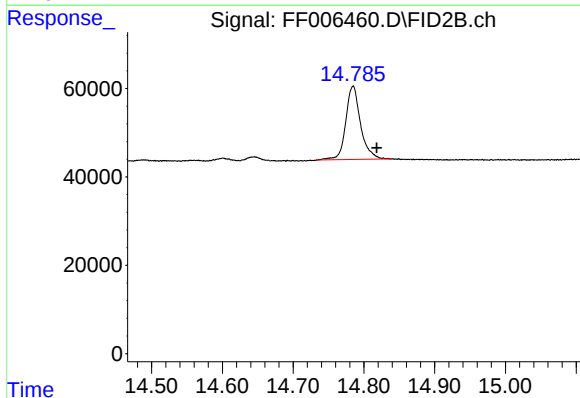


#10 N-TETRACOSANE

R.T.: 14.785 min
Delta R.T.: -0.033 min
Response: 239718
Conc: 1.72 ug/ml

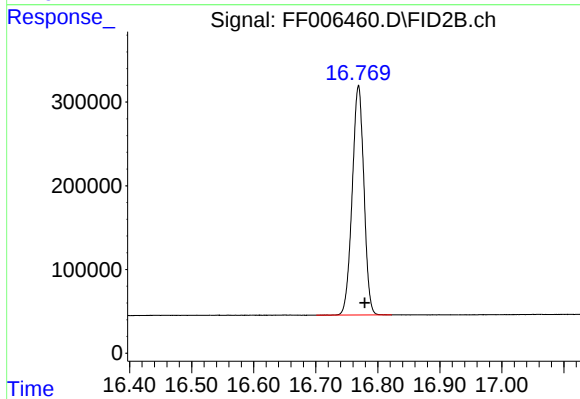

#12 N-OCTACOSANE


R.T.: 16.769 min
Delta R.T.: -0.010 min
Response: 3588307
Conc: 26.00 ug/ml

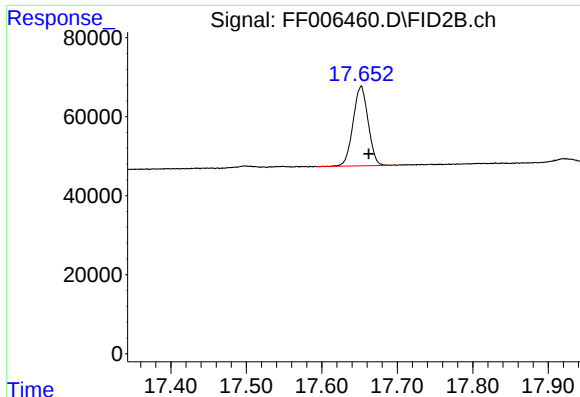

#13 N-TRIACONTANE


R.T.: 17.652 min
Delta R.T.: -0.010 min
Response: 279149
Conc: 2.02 ug/ml

Instrument :
FID_F
ClientSampleId :

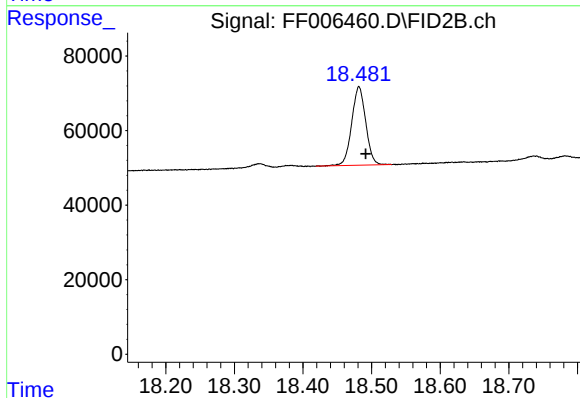


#14 N-DOTRIACONTANE

R.T.: 18.482 min
Delta R.T.: -0.010 min
Response: 299512
Conc: 2.28 ug/ml

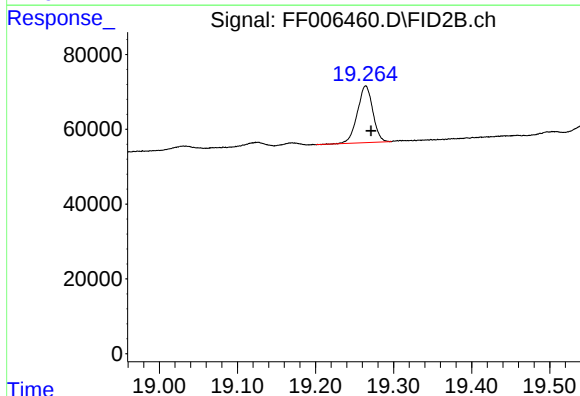

#15 N-TETRATRIACONTANE

R.T.: 19.264 min
Delta R.T.: -0.007 min
Response: 206848
Conc: 1.84 ug/ml

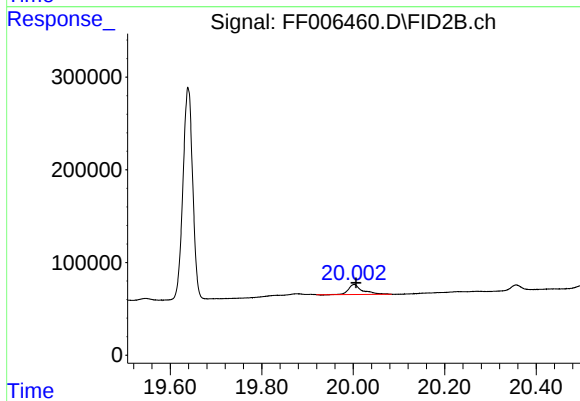

#16 N-HEXATRIACONTANE

R.T.: 20.002 min
Delta R.T.: -0.004 min
Response: 228217
Conc: 2.36 ug/ml