

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
 Data File : FF006461.D
 Signal(s) : FID2B.ch
 Acq On : 24 Feb 2020 13:18
 Operator : DD\AJ
 Sample : L1624-01 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 25 00:29:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.601	966333	7.932 ug/ml
Target Compounds			
7) N-EICOSANE	12.511	99968	0.709 ug/ml
10) N-TETRACOSANE	14.785	431809	3.090 ug/ml
11) N-HEXACOSANE	15.820	99480	0.721 ug/ml
12) N-OCTACOSANE	16.768	240509	1.743 ug/ml
13) N-TRIACONTANE	17.652	301915	2.183 ug/ml
14) N-DOTRIACONTANE	18.480	163849	1.245 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
Data File : FF006461.D
Signal(s) : FID2B.ch
Acq On : 24 Feb 2020 13:18
Operator : DD\AJ
Sample : L1624-01 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 25 00:29:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

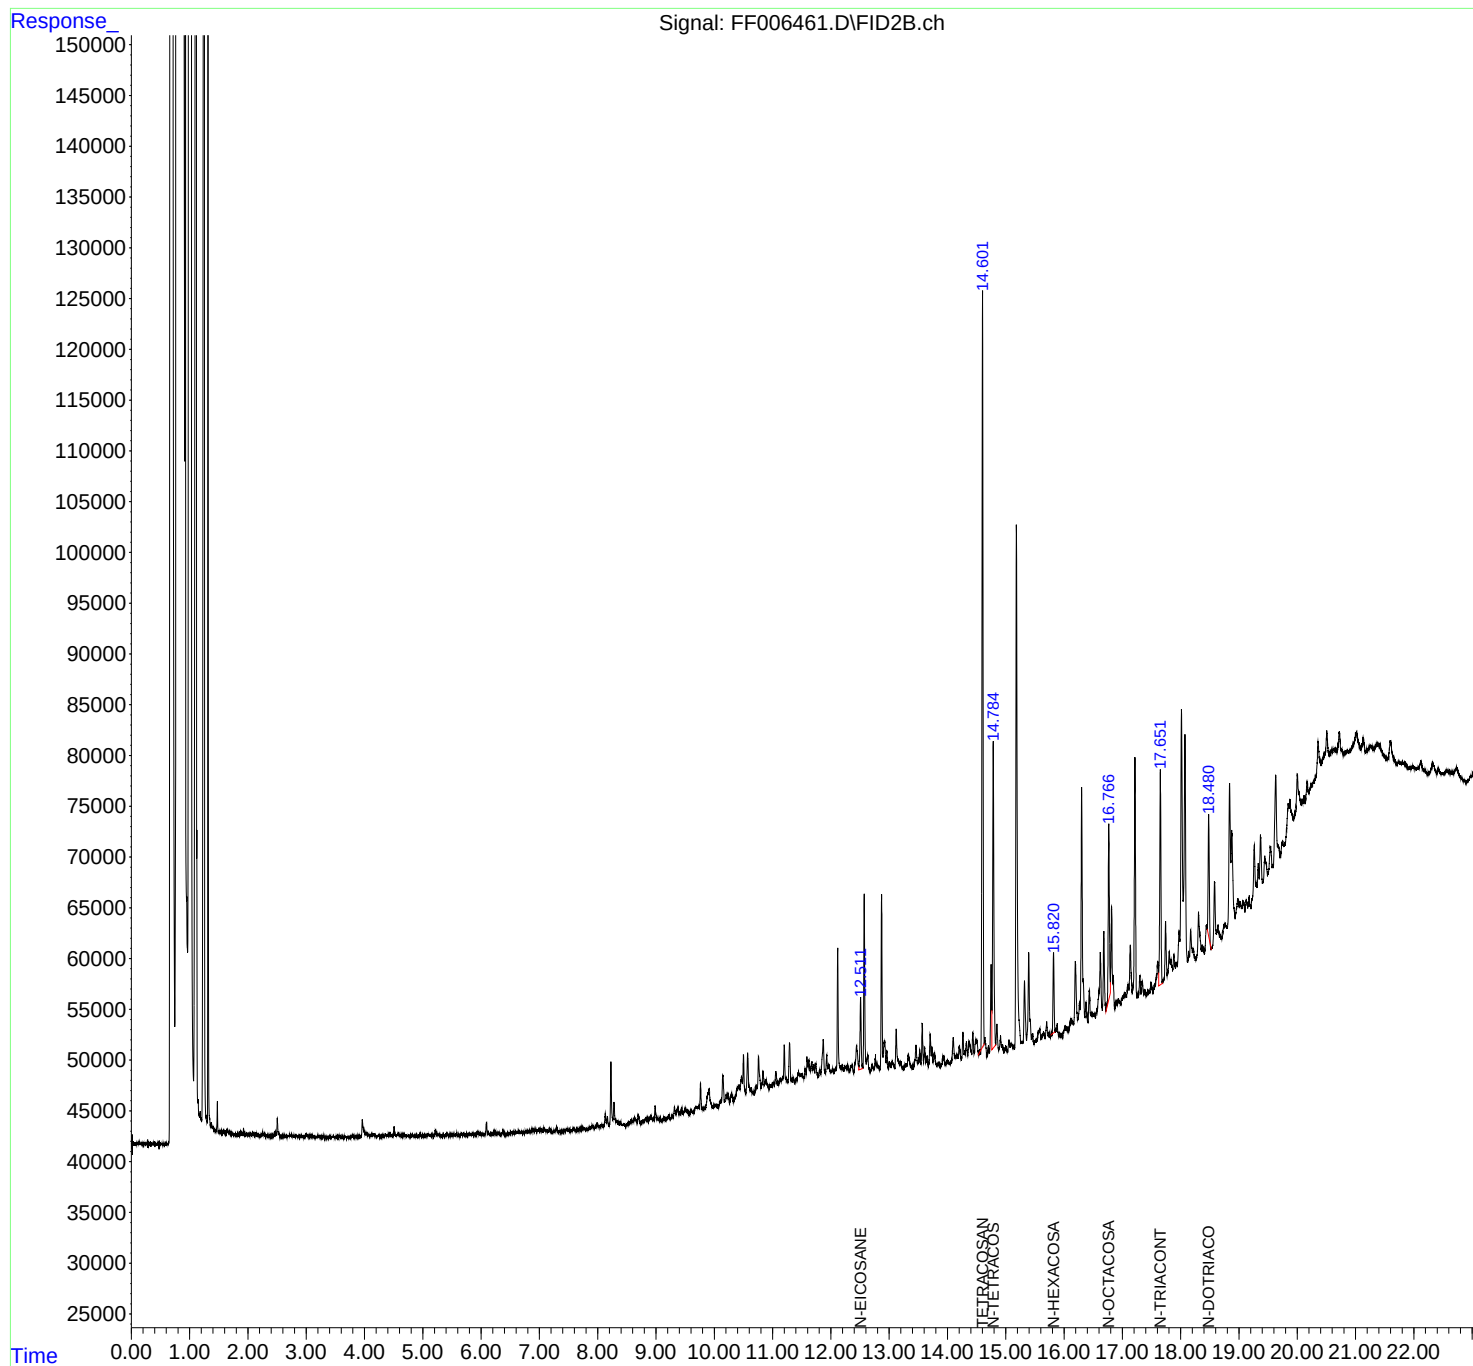


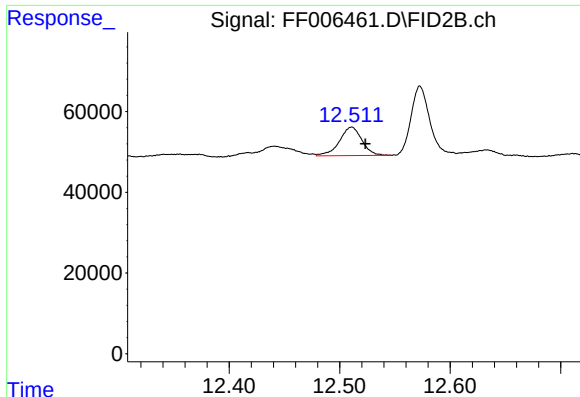

#7 N-EICOSANE


R.T.: 12.511 min
Delta R.T.: -0.012 min
Response: 99968
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :

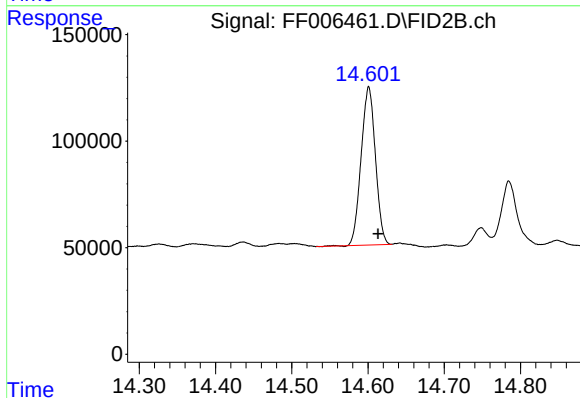


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.601 min
Delta R.T.: -0.012 min
Response: 966333
Conc: 7.93 ug/ml

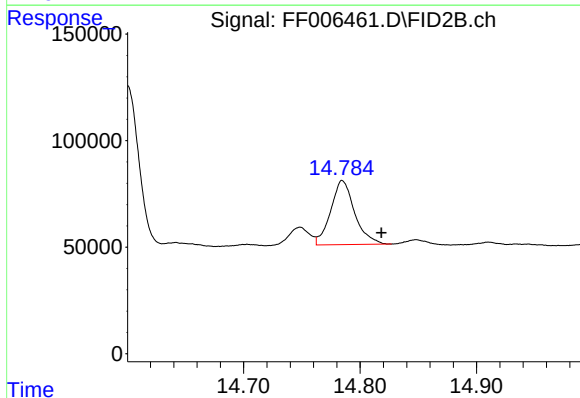


#10 N-TETRACOSANE

R.T.: 14.785 min
Delta R.T.: -0.033 min
Response: 431809
Conc: 3.09 ug/ml

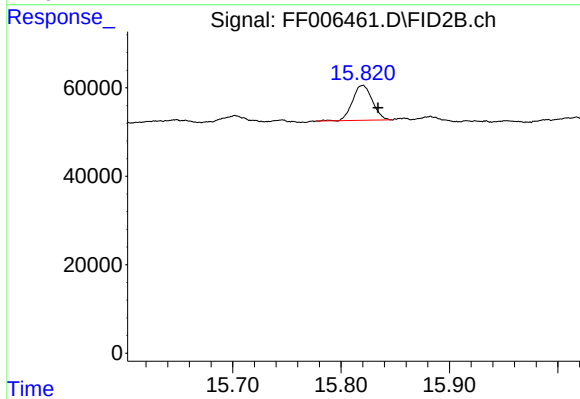

#11 N-HEXACOSANE


R.T.: 15.820 min
Delta R.T.: -0.014 min
Response: 99480
Conc: 0.72 ug/ml

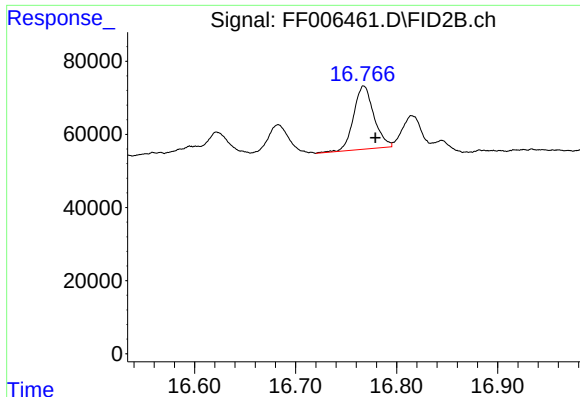

#12 N-OCTACOSANE


R.T.: 16.768 min
Delta R.T.: -0.011 min
Response: 240509
Conc: 1.74 ug/ml

Instrument :
FID_F
ClientSampleId :

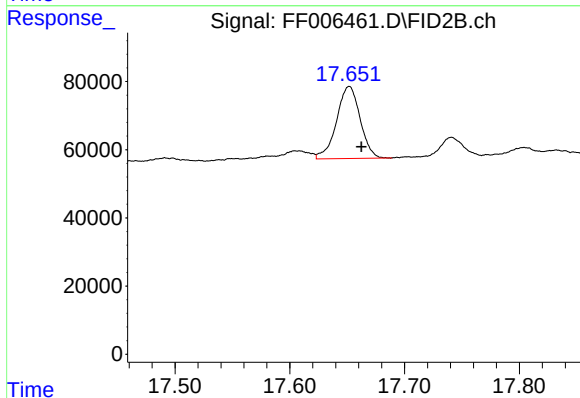

#13 N-TRIACONTANE

R.T.: 17.652 min
Delta R.T.: -0.011 min
Response: 301915
Conc: 2.18 ug/ml

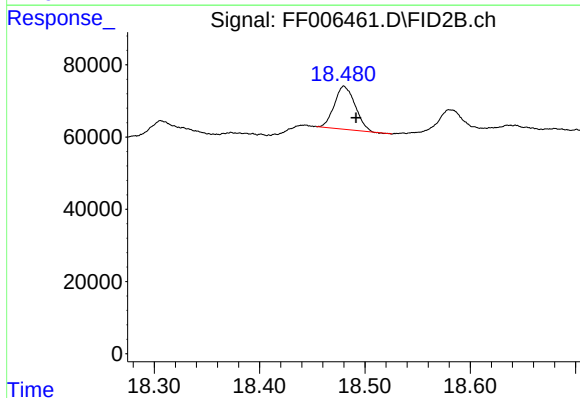

#14 N-DOTRIACONTANE

R.T.: 18.480 min
Delta R.T.: -0.011 min
Response: 163849
Conc: 1.25 ug/ml