

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
 Data File : FF006462.D
 Signal(s) : FID2B.ch
 Acq On : 24 Feb 2020 13:48
 Operator : DD\AJ
 Sample : L1603-02 2X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 25 00:29:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.602	1546867	12.697 ug/ml
Target Compounds			
4) N-TETRADECANE	8.233	85998	0.625 ug/ml
10) N-TETRACOSANE	14.787	151517	1.084 ug/ml
11) N-HEXACOSANE	15.822	102728	0.744 ug/ml
12) N-OCTACOSANE	16.767	326843	2.368 ug/ml
13) N-TRIACONTANE	17.652	381636	2.760 ug/ml
14) N-DOTRIACONTANE	18.480	305036	2.319 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
Data File : FF006462.D
Signal(s) : FID2B.ch
Acq On : 24 Feb 2020 13:48
Operator : DD\AJ
Sample : L1603-02 2X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 25 00:29:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

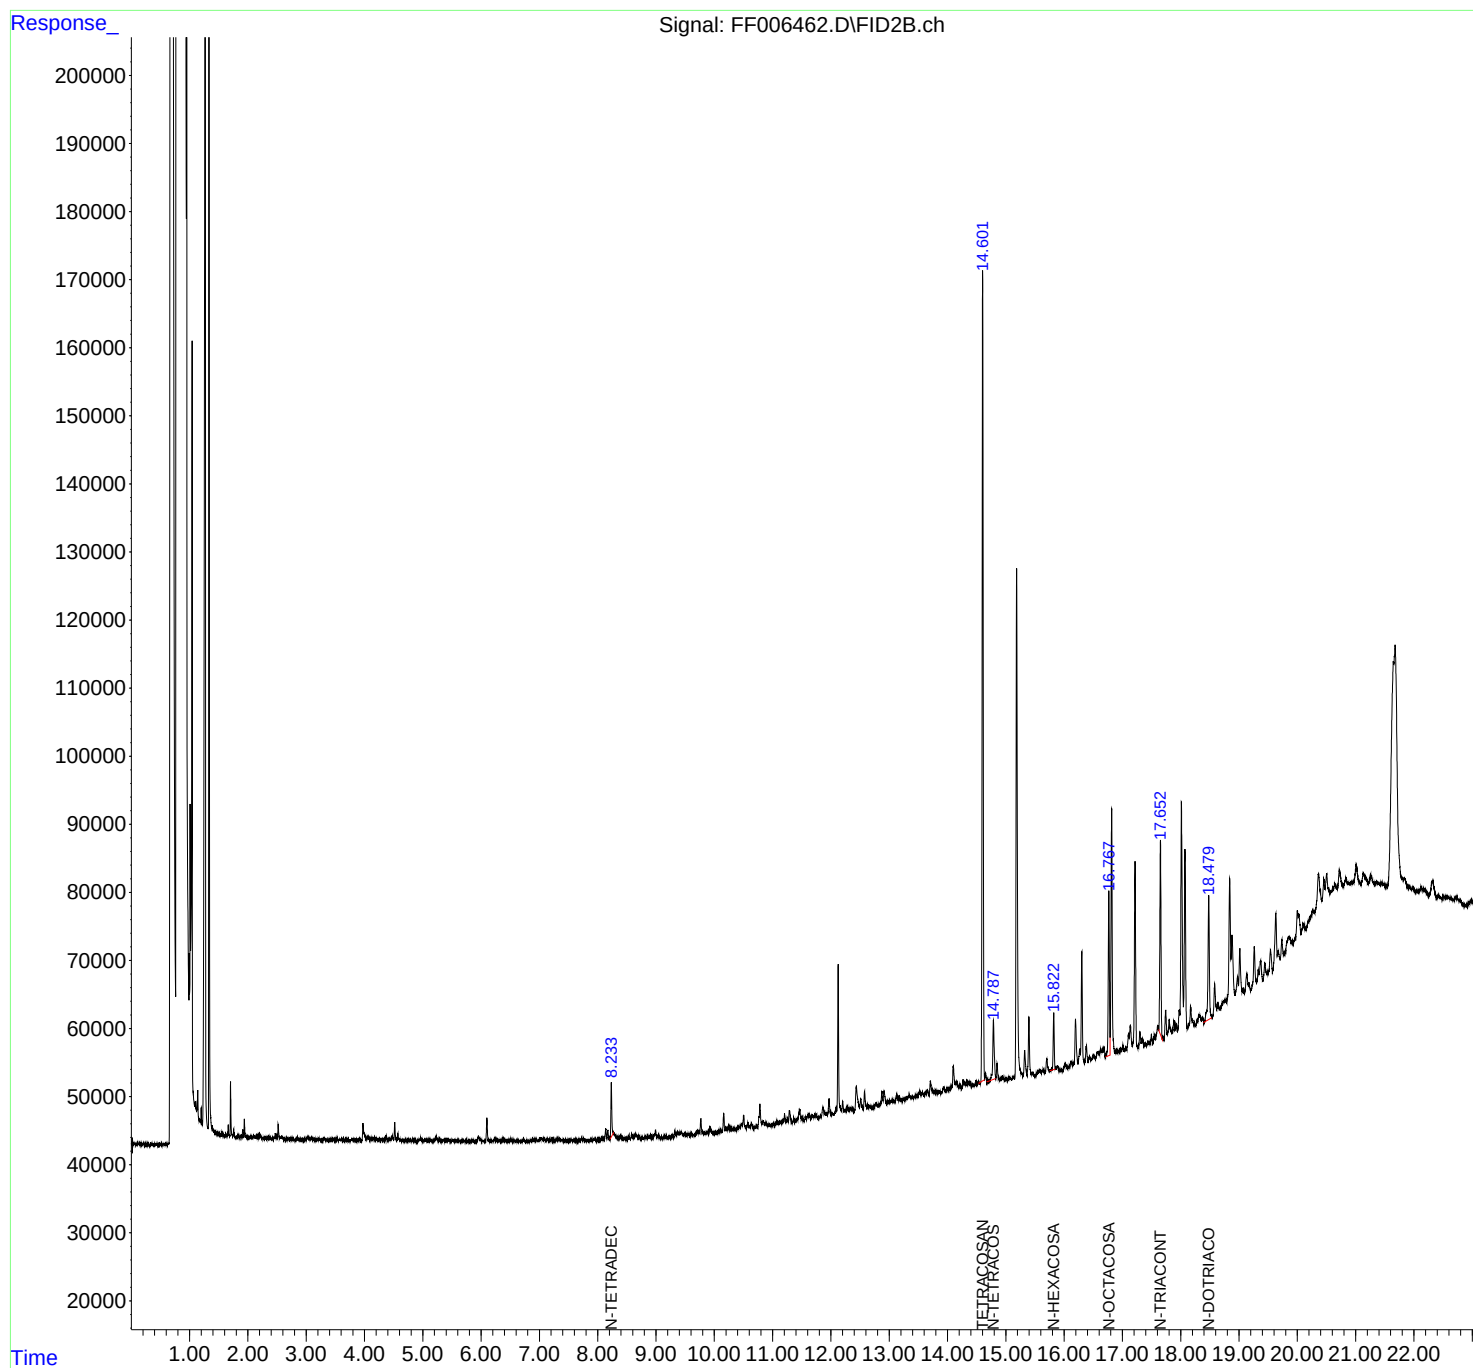


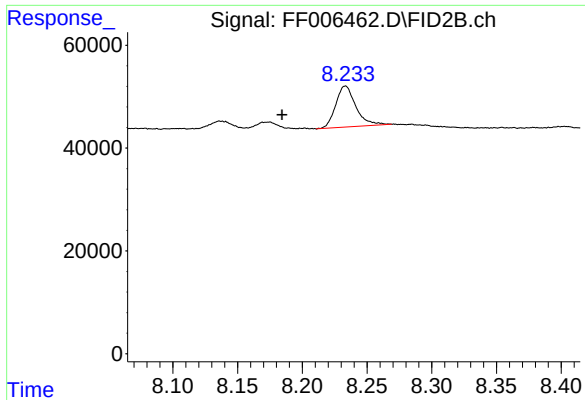

#4 N-TETRADECANE


R.T.: 8.233 min
Delta R.T.: 0.049 min
Response: 85998
Conc: 0.63 ug/ml

Instrument :
FID_F
ClientSampleId :

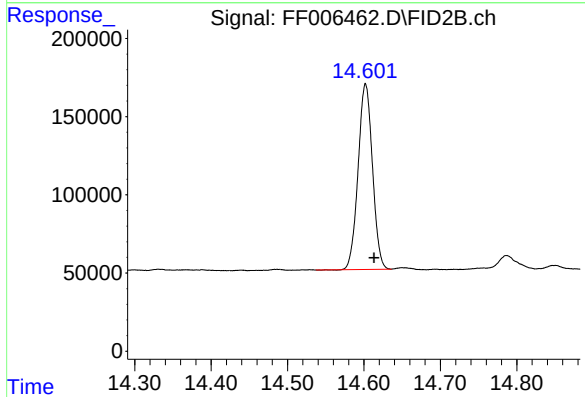


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.602 min
Delta R.T.: -0.011 min
Response: 1546867
Conc: 12.70 ug/ml

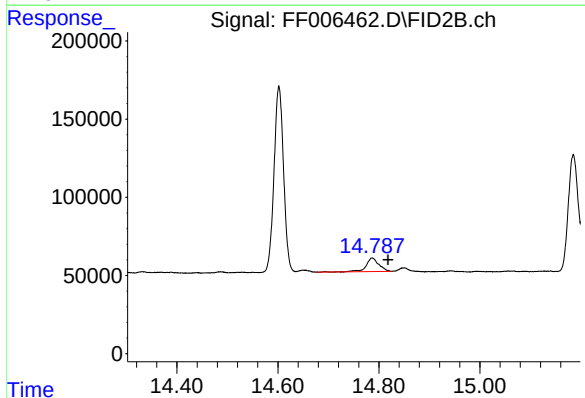


#10 N-TETRACOSANE

R.T.: 14.787 min
Delta R.T.: -0.032 min
Response: 151517
Conc: 1.08 ug/ml

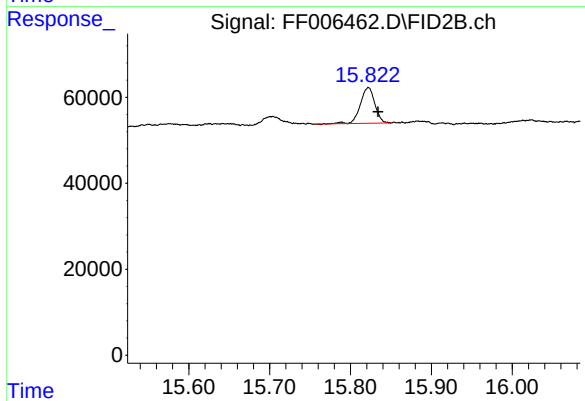

#11 N-HEXACOSANE


R.T.: 15.822 min
Delta R.T.: -0.012 min
Response: 102728
Conc: 0.74 ug/ml

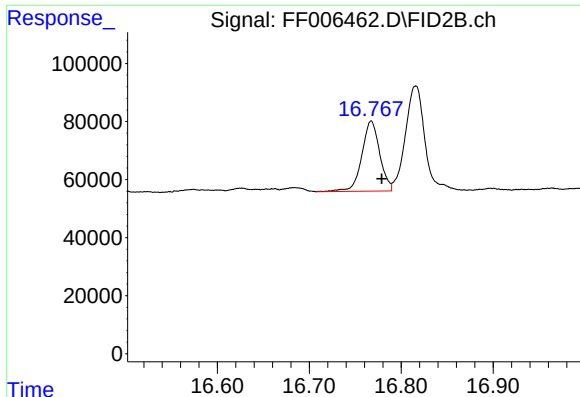

#12 N-OCTACOSANE


R.T.: 16.767 min
Delta R.T.: -0.011 min
Response: 326843
Conc: 2.37 ug/ml

Instrument :
FID_F
ClientSampleId :

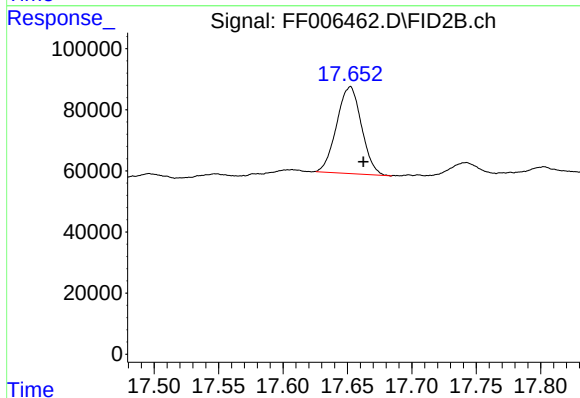

#13 N-TRIACONTANE

R.T.: 17.652 min
Delta R.T.: -0.010 min
Response: 381636
Conc: 2.76 ug/ml

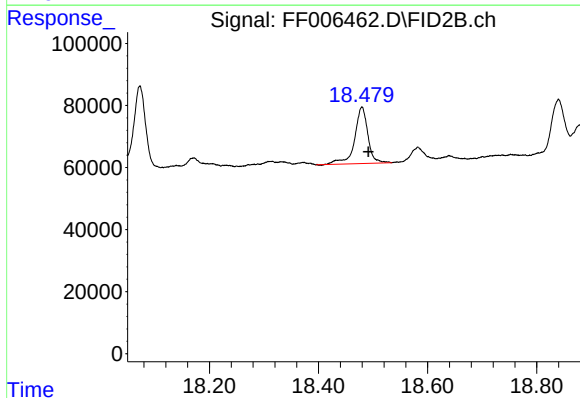

#14 N-DOTRIACONTANE

R.T.: 18.480 min
Delta R.T.: -0.012 min
Response: 305036
Conc: 2.32 ug/ml