

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
 Data File : FF006463.D
 Signal(s) : FID2B.ch
 Acq On : 24 Feb 2020 14:49
 Operator : DD\AJ
 Sample : L1605-01 2X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 25 00:29:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.605	1119421	9.188 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.788	127429	0.912 ug/ml
12) N-OCTACOSANE	16.767	187149	1.356 ug/ml
13) N-TRIACONTANE	17.651	274070	1.982 ug/ml
14) N-DOTRIACONTANE	18.479	213689	1.624 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
Data File : FF006463.D
Signal(s) : FID2B.ch
Acq On : 24 Feb 2020 14:49
Operator : DD\AJ
Sample : L1605-01 2X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 25 00:29:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

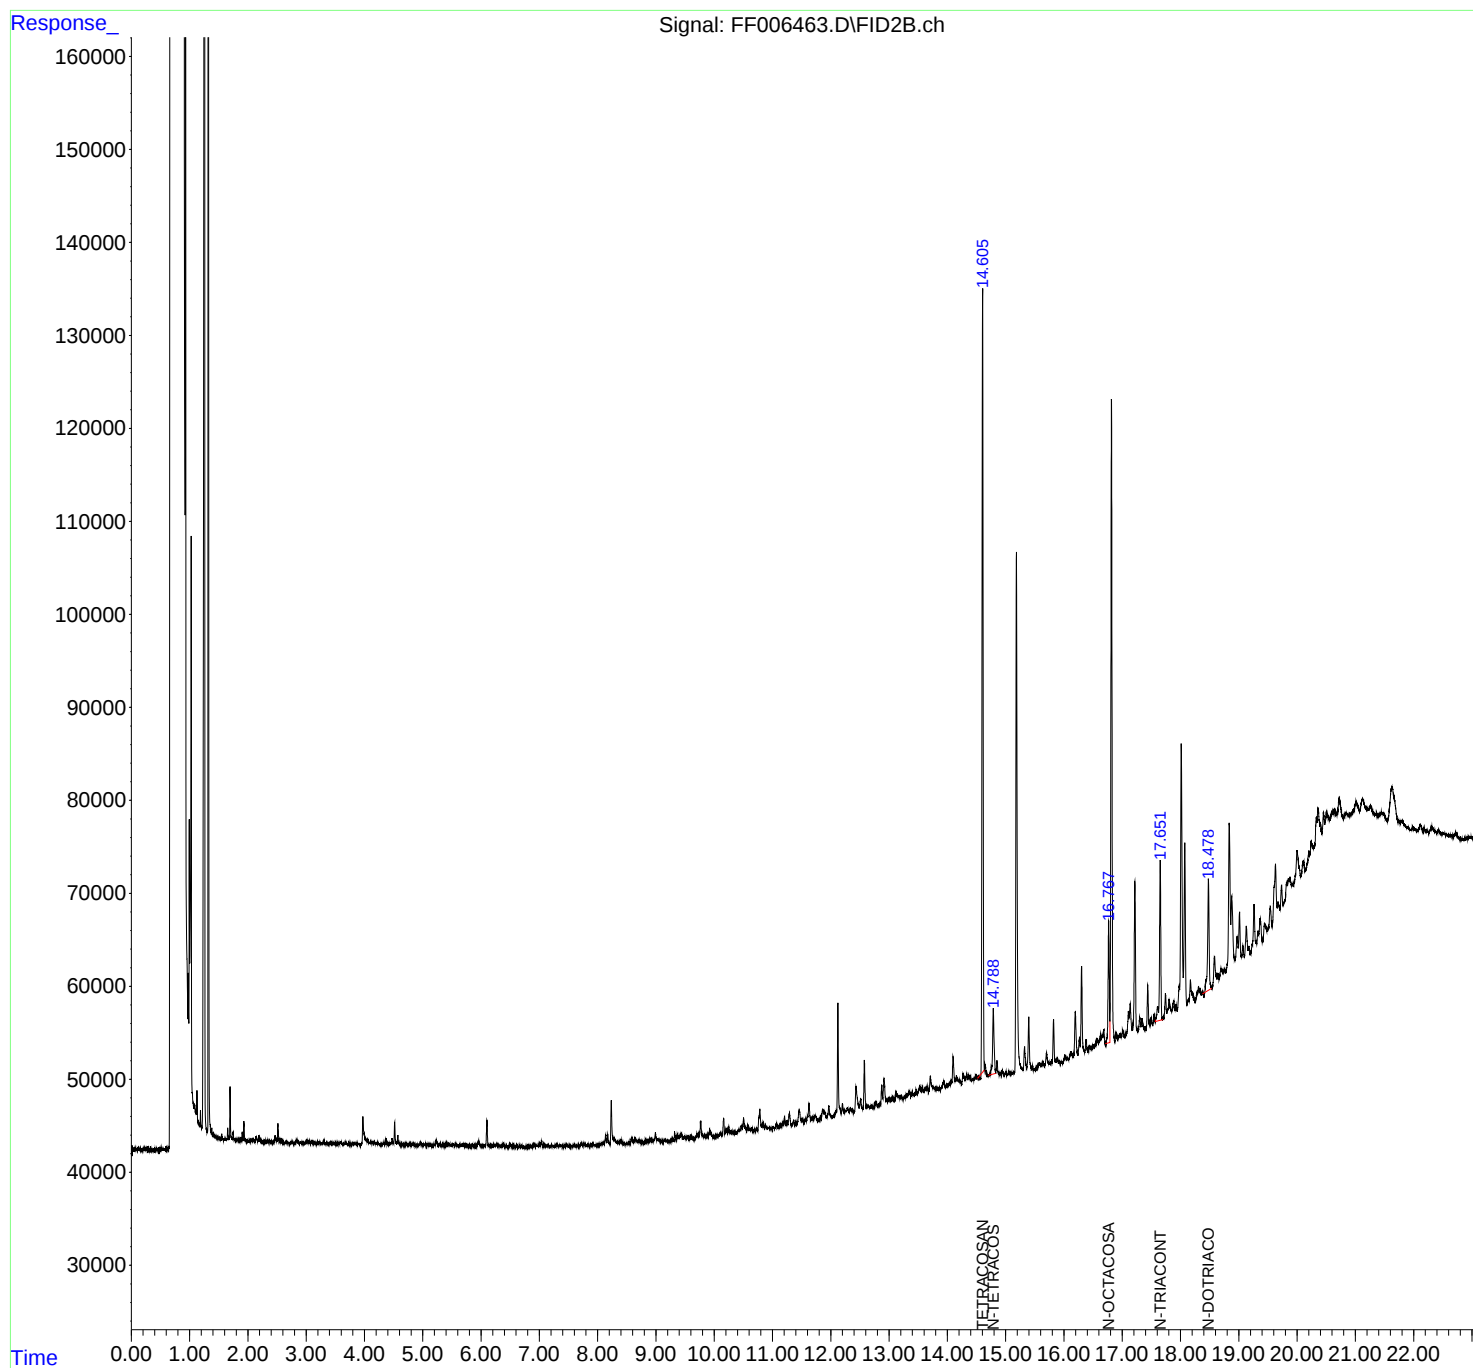


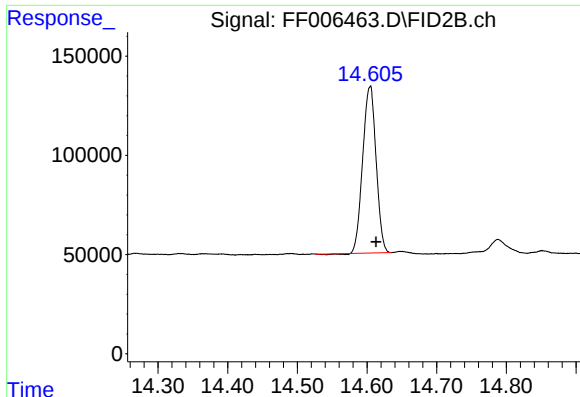

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.605 min
Delta R.T.: -0.009 min
Response: 1119421
Conc: 9.19 ug/ml

Instrument :
FID_F
ClientSampleId :

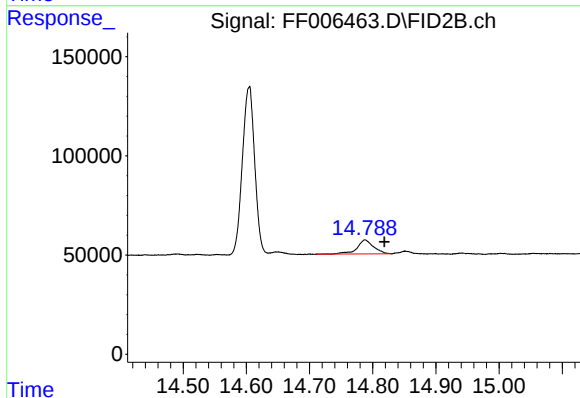


#10 N-TETRACOSANE

R.T.: 14.788 min
Delta R.T.: -0.030 min
Response: 127429
Conc: 0.91 ug/ml

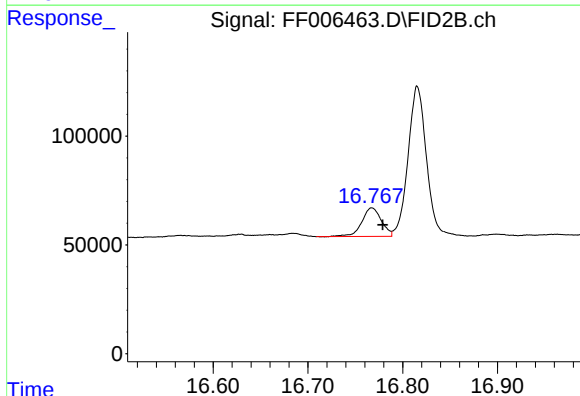


#12 N-OCTACOSANE

R.T.: 16.767 min
Delta R.T.: -0.011 min
Response: 187149
Conc: 1.36 ug/ml

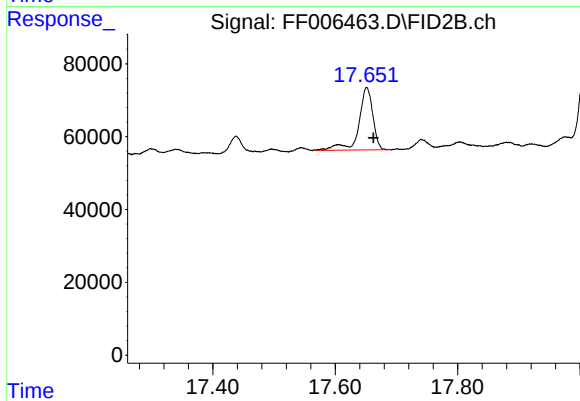

#13 N-TRIACONTANE

R.T.: 17.651 min
Delta R.T.: -0.011 min
Response: 274070
Conc: 1.98 ug/ml

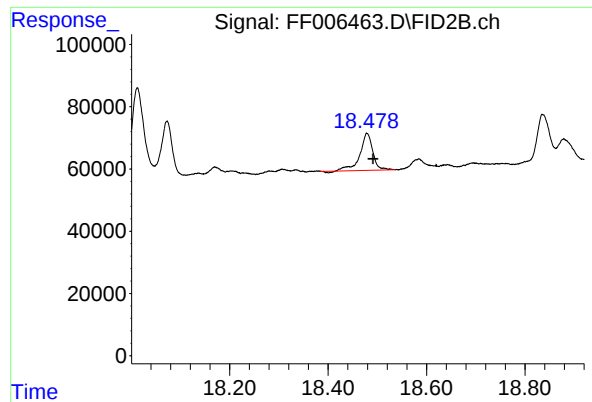

#14 N-DOTRIACONTANE

R.T.: 18.479 min
Delta R.T.: -0.012 min
Response: 213689
Conc: 1.62 ug/ml

Instrument :
FID_F
ClientSampleId :