

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
 Data File : FF006464.D
 Signal(s) : FID2B.ch
 Acq On : 24 Feb 2020 15:19
 Operator : DD\AJ
 Sample : L1605-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Feb 25 00:29:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.604	2319955	19.043 ug/ml
Target Compounds			
4) N-TETRADECANE	8.234	115123	0.837 ug/ml
7) N-EICOSANE	12.577f	132554	0.941 ug/ml
10) N-TETRACOSANE	14.789	180928	1.295 ug/ml
11) N-HEXACOSANE	15.824	103968	0.753 ug/ml
12) N-OCTACOSANE	16.770	348662	2.526 ug/ml
13) N-TRIACONTANE	17.652	444060	3.211 ug/ml
14) N-DOTRIACONTANE	18.480	449610	3.417 ug/ml
15) N-TETRATRIACONTANE	19.262	136749	1.218 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022420\
Data File : FF006464.D
Signal(s) : FID2B.ch
Acq On : 24 Feb 2020 15:19
Operator : DD\AJ
Sample : L1605-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 25 00:29:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

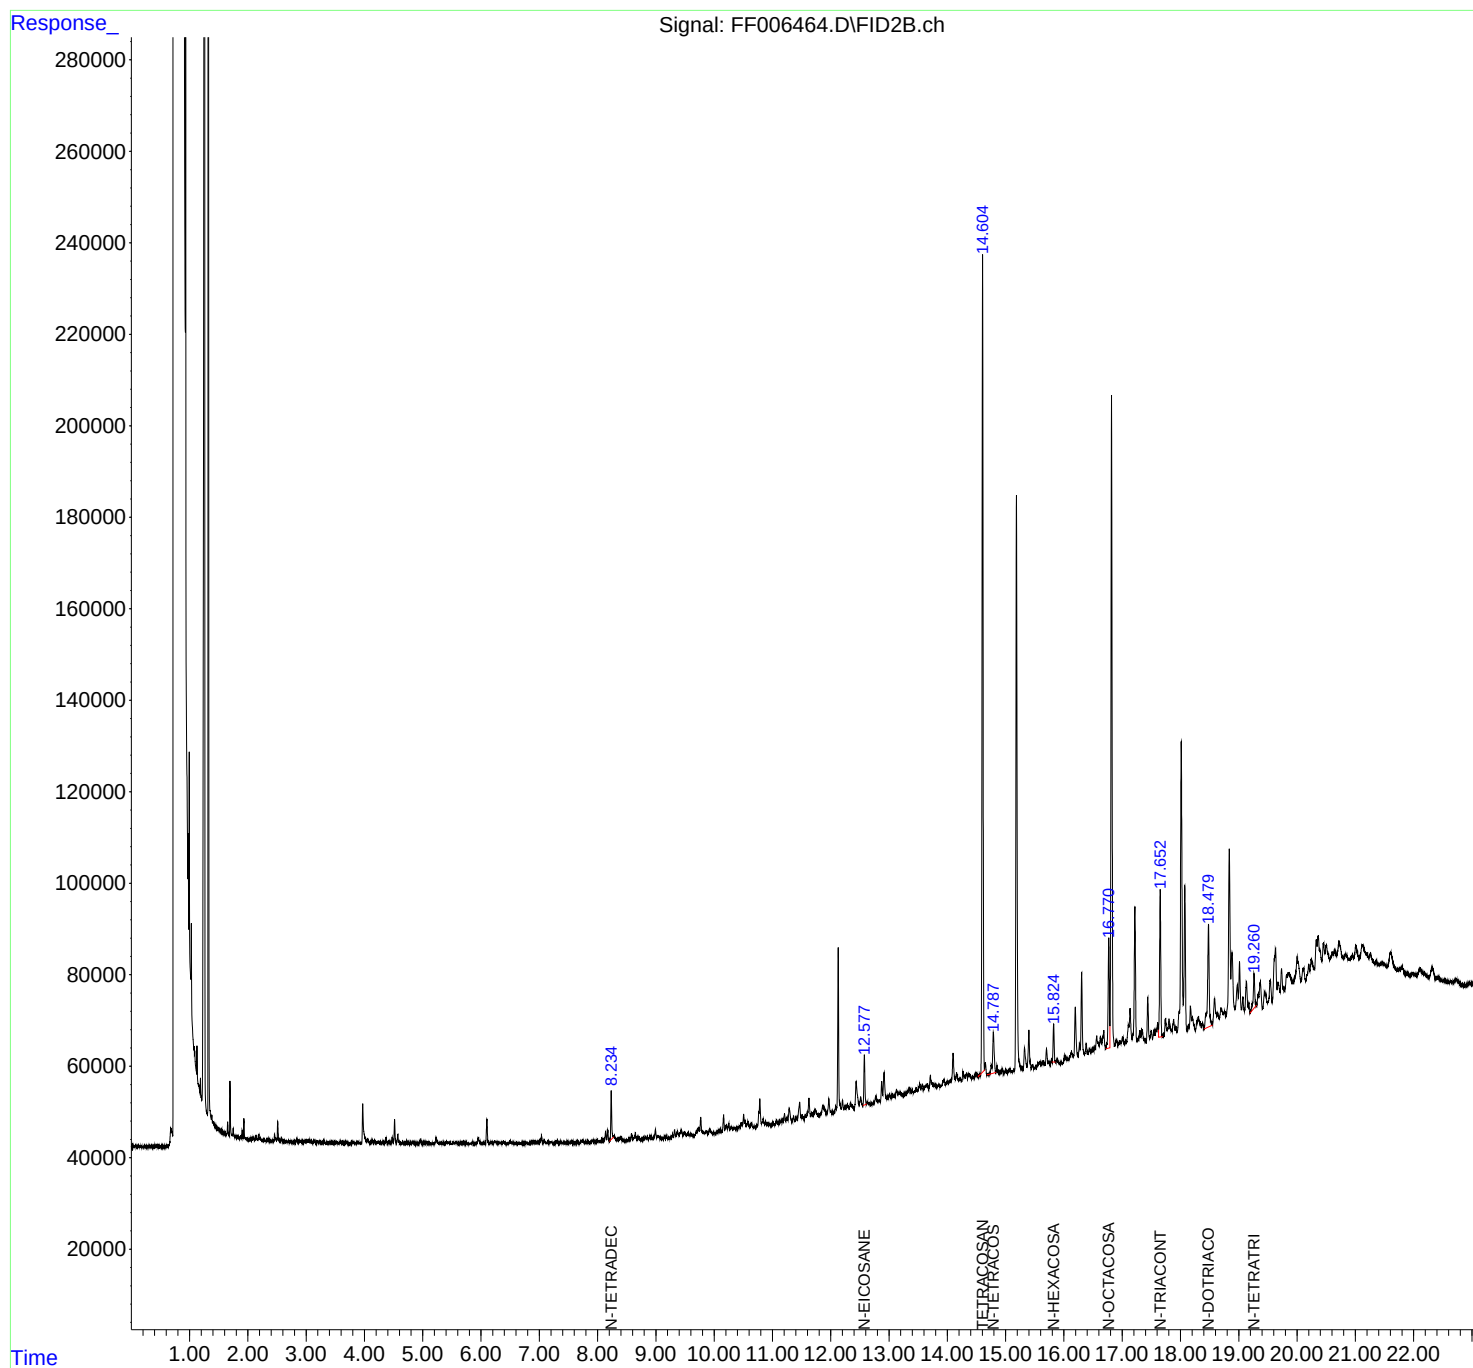


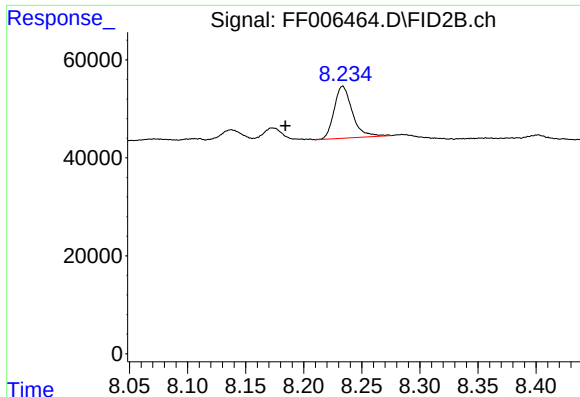

#4 N-TETRADECANE


R.T.: 8.234 min
Delta R.T.: 0.049 min
Response: 115123
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :

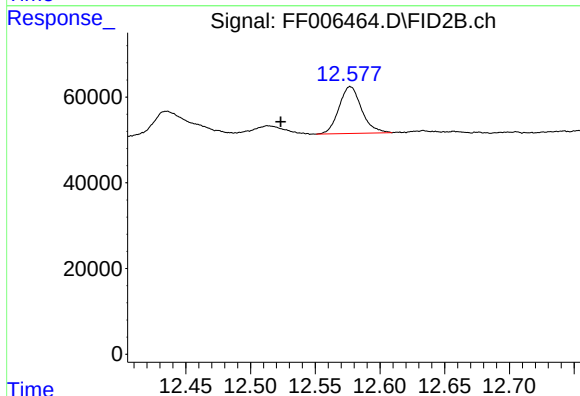


#7 N-EICOSANE

R.T.: 12.577 min
Delta R.T.: 0.054 min
Response: 132554
Conc: 0.94 ug/ml

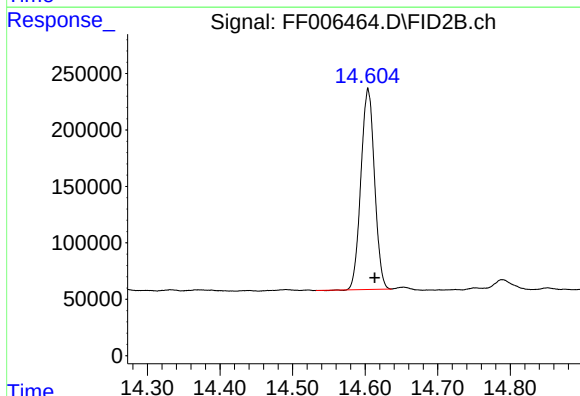


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.604 min
Delta R.T.: -0.009 min
Response: 2319955
Conc: 19.04 ug/ml

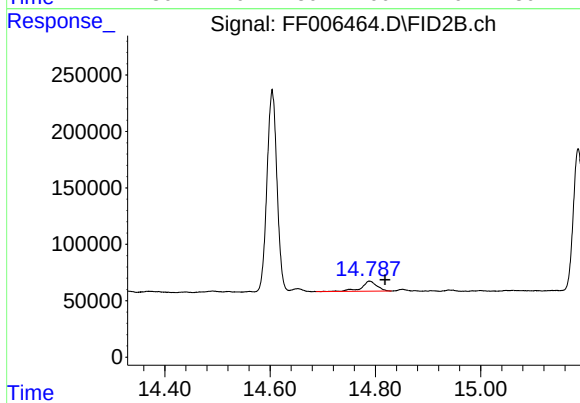

#10 N-TETRACOSANE


R.T.: 14.789 min
Delta R.T.: -0.029 min
Response: 180928
Conc: 1.29 ug/ml

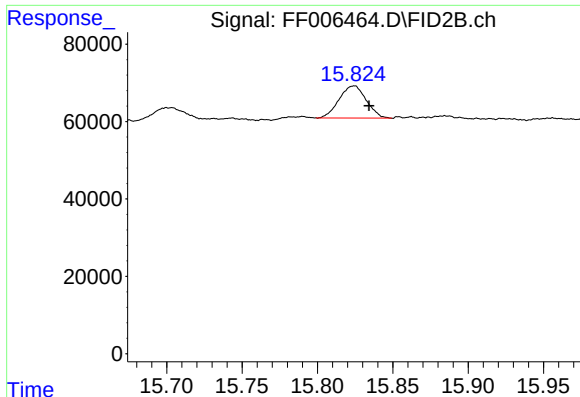

#11 N-HEXACOSANE


R.T.: 15.824 min
Delta R.T.: -0.010 min
Response: 103968
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :

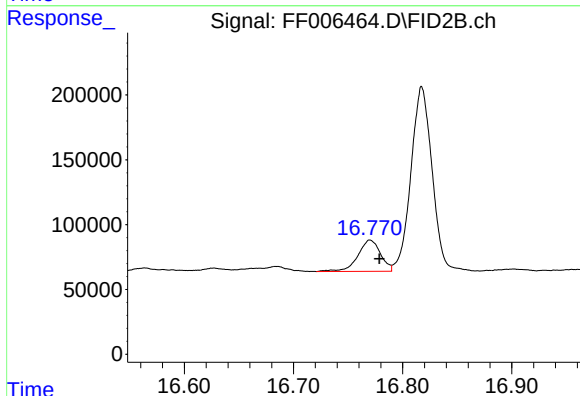


#12 N-OCTACOSANE

R.T.: 16.770 min
Delta R.T.: -0.009 min
Response: 348662
Conc: 2.53 ug/ml

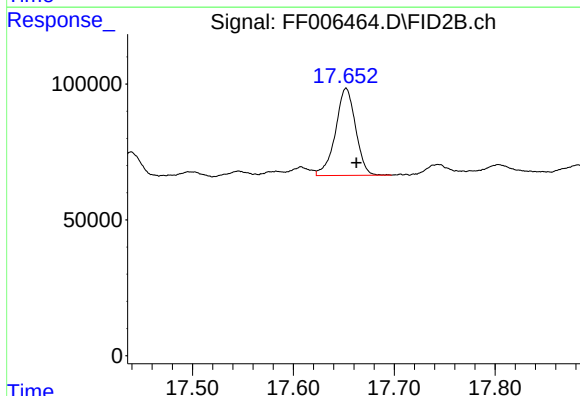


#13 N-TRIACONTANE

R.T.: 17.652 min
Delta R.T.: -0.010 min
Response: 444060
Conc: 3.21 ug/ml

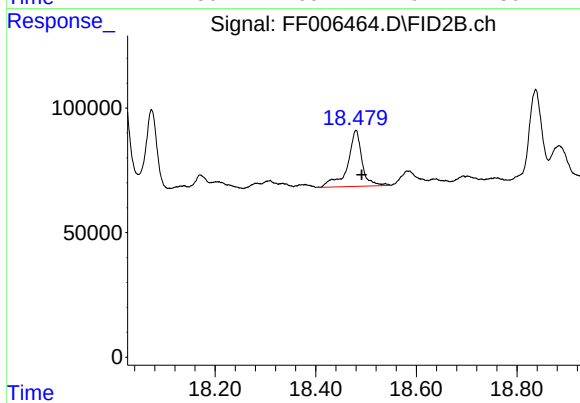

#14 N-DOTRIACONTANE

R.T.: 18.480 min
Delta R.T.: -0.011 min
Response: 449610
Conc: 3.42 ug/ml

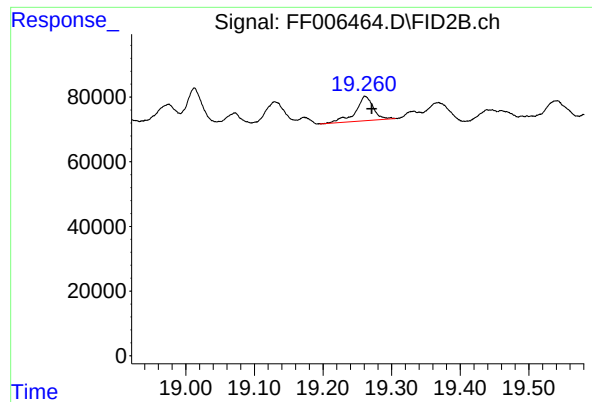

#15 N-TETRATRIACONTANE

R.T.: 19.262 min
Delta R.T.: -0.010 min
Response: 136749
Conc: 1.22 ug/ml

Instrument :
FID_F
ClientSampleId :