

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022725\
Data File : FF015562.D
Signal(s) : FID2B.ch
Acq On : 27 Feb 2025 18:18
Operator : YP\AJ
Sample : Q1449-02 10X
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 00:44:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021025.M
Quant Title :
QLast Update : Mon Feb 10 16:23:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.022	199721	1.812 ug/ml
Target Compounds			
18) N-TETRACONTANE	22.155	191439	2.056 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF022725\
Data File : FF015562.D
Signal(s) : FID2B.ch
Acq On : 27 Feb 2025 18:18
Operator : YP\AJ
Sample : Q1449-02 10X
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 00:44:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021025.M
Quant Title :
QLast Update : Mon Feb 10 16:23:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

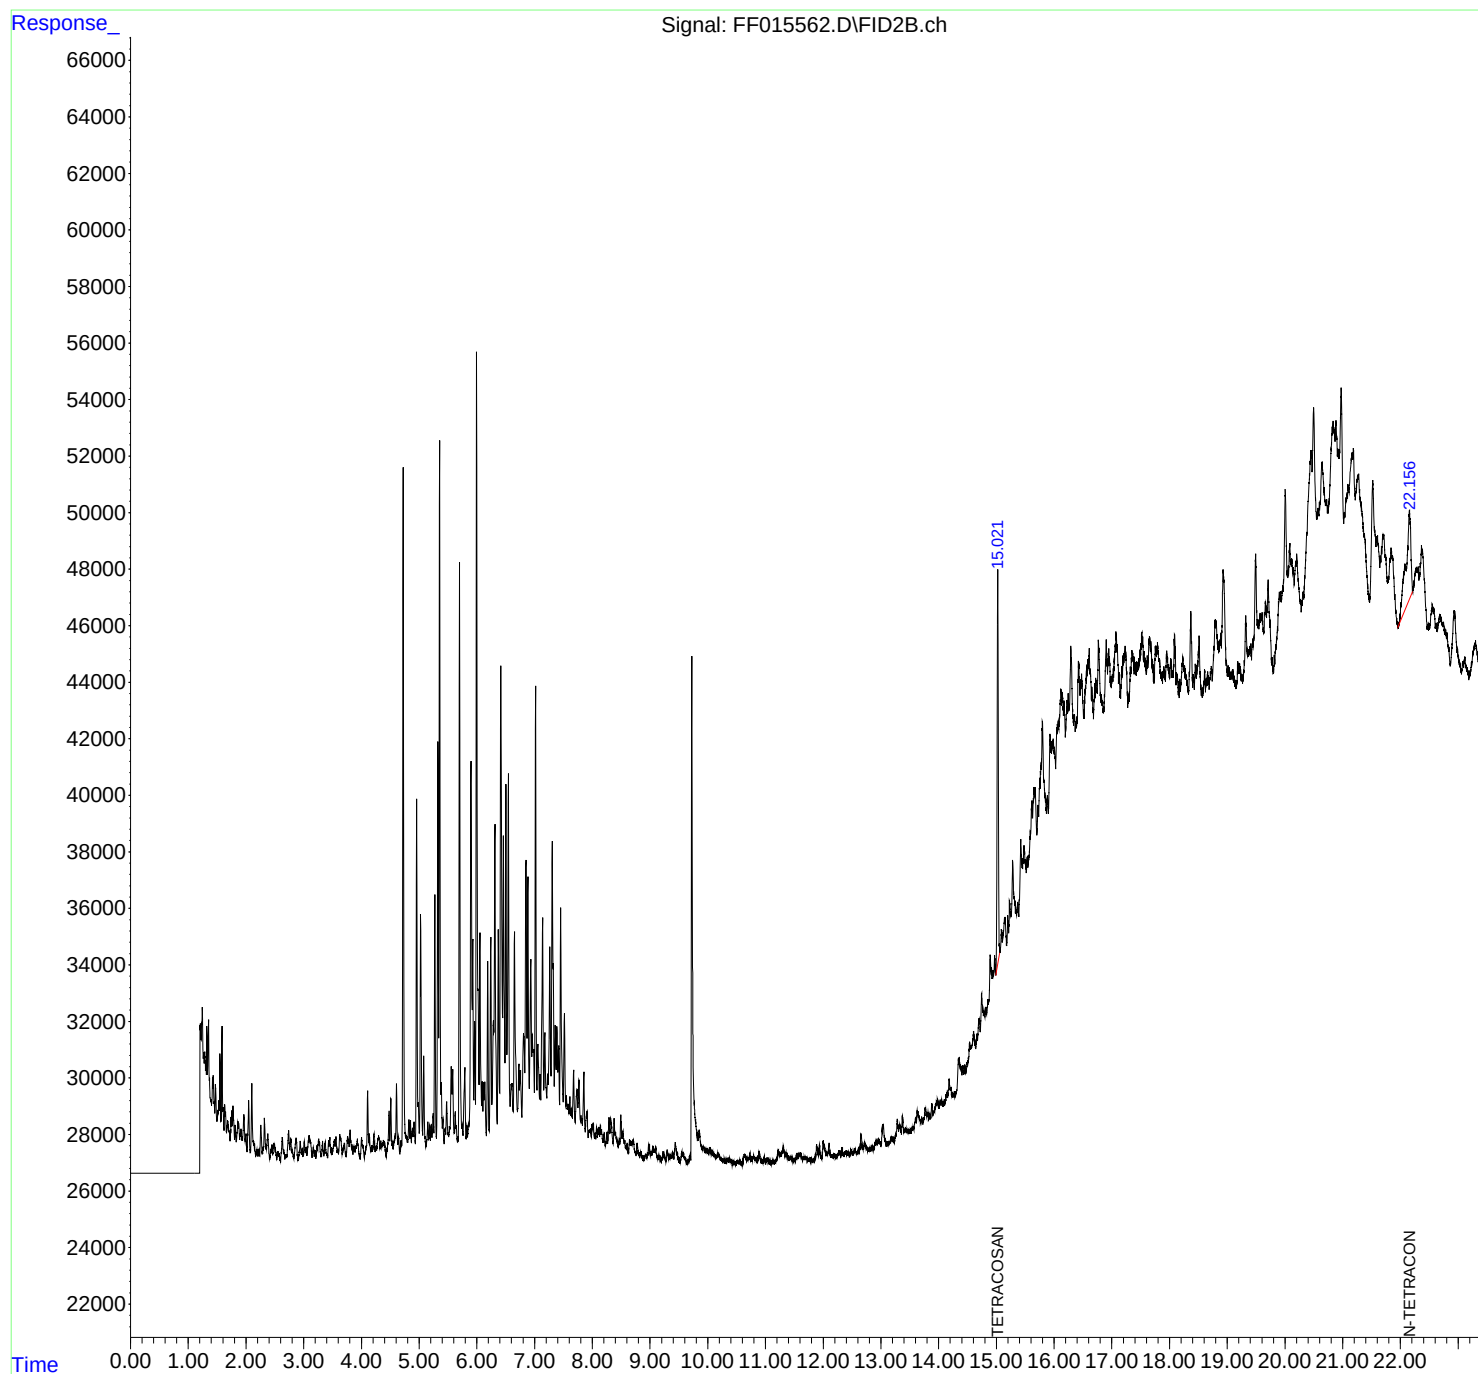


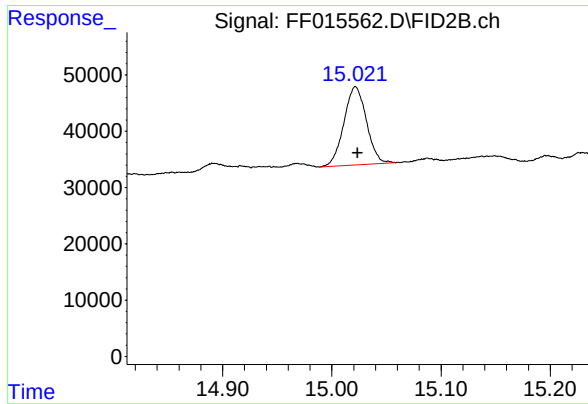

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.022 min
Delta R.T.: -0.002 min
Response: 199721
Conc: 1.81 ug/ml

Instrument :
FID_F
ClientSampleId :

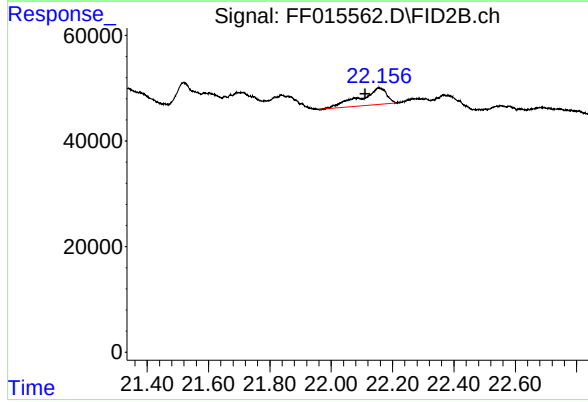

#18 N-TETRACONTANE

R.T.: 22.155 min
Delta R.T.: 0.044 min
Response: 191439
Conc: 2.06 ug/ml