

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030119\
 Data File : FF003671.D
 Signal(s) : FID2B.ch
 Acq On : 01 Mar 2019 14:41
 Operator : AJ\SJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 TRPH STD

Integration File: autoint1.e
 Quant Time: Mar 04 08:31:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:29:28 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.598	6247747	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.228	6930006	50.000 ug/ml
2) N-DECANE	4.321	7005449	50.000 ug/ml
3) N-DODECANE	6.344	7139156	50.000 ug/ml
4) N-TETRADECANE	8.138	7339427	50.000 ug/ml
5) N-HEXADECANE	9.740	7359712	50.000 ug/ml
6) N-OCTADECANE	11.184	7416987	50.000 ug/ml
7) N-EICOSANE	12.496	7329189	50.000 ug/ml
8) N-DOCOSANE	13.697	7228416	50.000 ug/ml
10) N-TETRACOSANE	14.802	7094457	50.000 ug/ml
11) N-HEXACOSANE	15.827	6933857	50.000 ug/ml
12) N-OCTACOSANE	16.780	6752974	50.000 ug/ml
13) N-TRIACONTANE	17.671	6557888	50.000 ug/ml
14) N-DOTRIACONTANE	18.507	6289687	50.000 ug/ml
15) N-TETRATRIACONTANE	19.294	6013989	50.000 ug/ml
16) N-HEXATRIACONTANE	20.038	5868202	50.000 ug/ml
17) N-OCTATRIACONTANE	20.772	5226401	50.000 ug/ml
18) N-TETRACONTANE	21.659	5584387	50.000 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030119\
Data File : FF003671.D
Signal(s) : FID2B.ch
Acq On : 01 Mar 2019 14:41
Operator : AJ\SJ
Sample : 50 TRPH STD
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

Integration File: autoint1.e
Quant Time: Mar 04 08:31:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:29:28 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

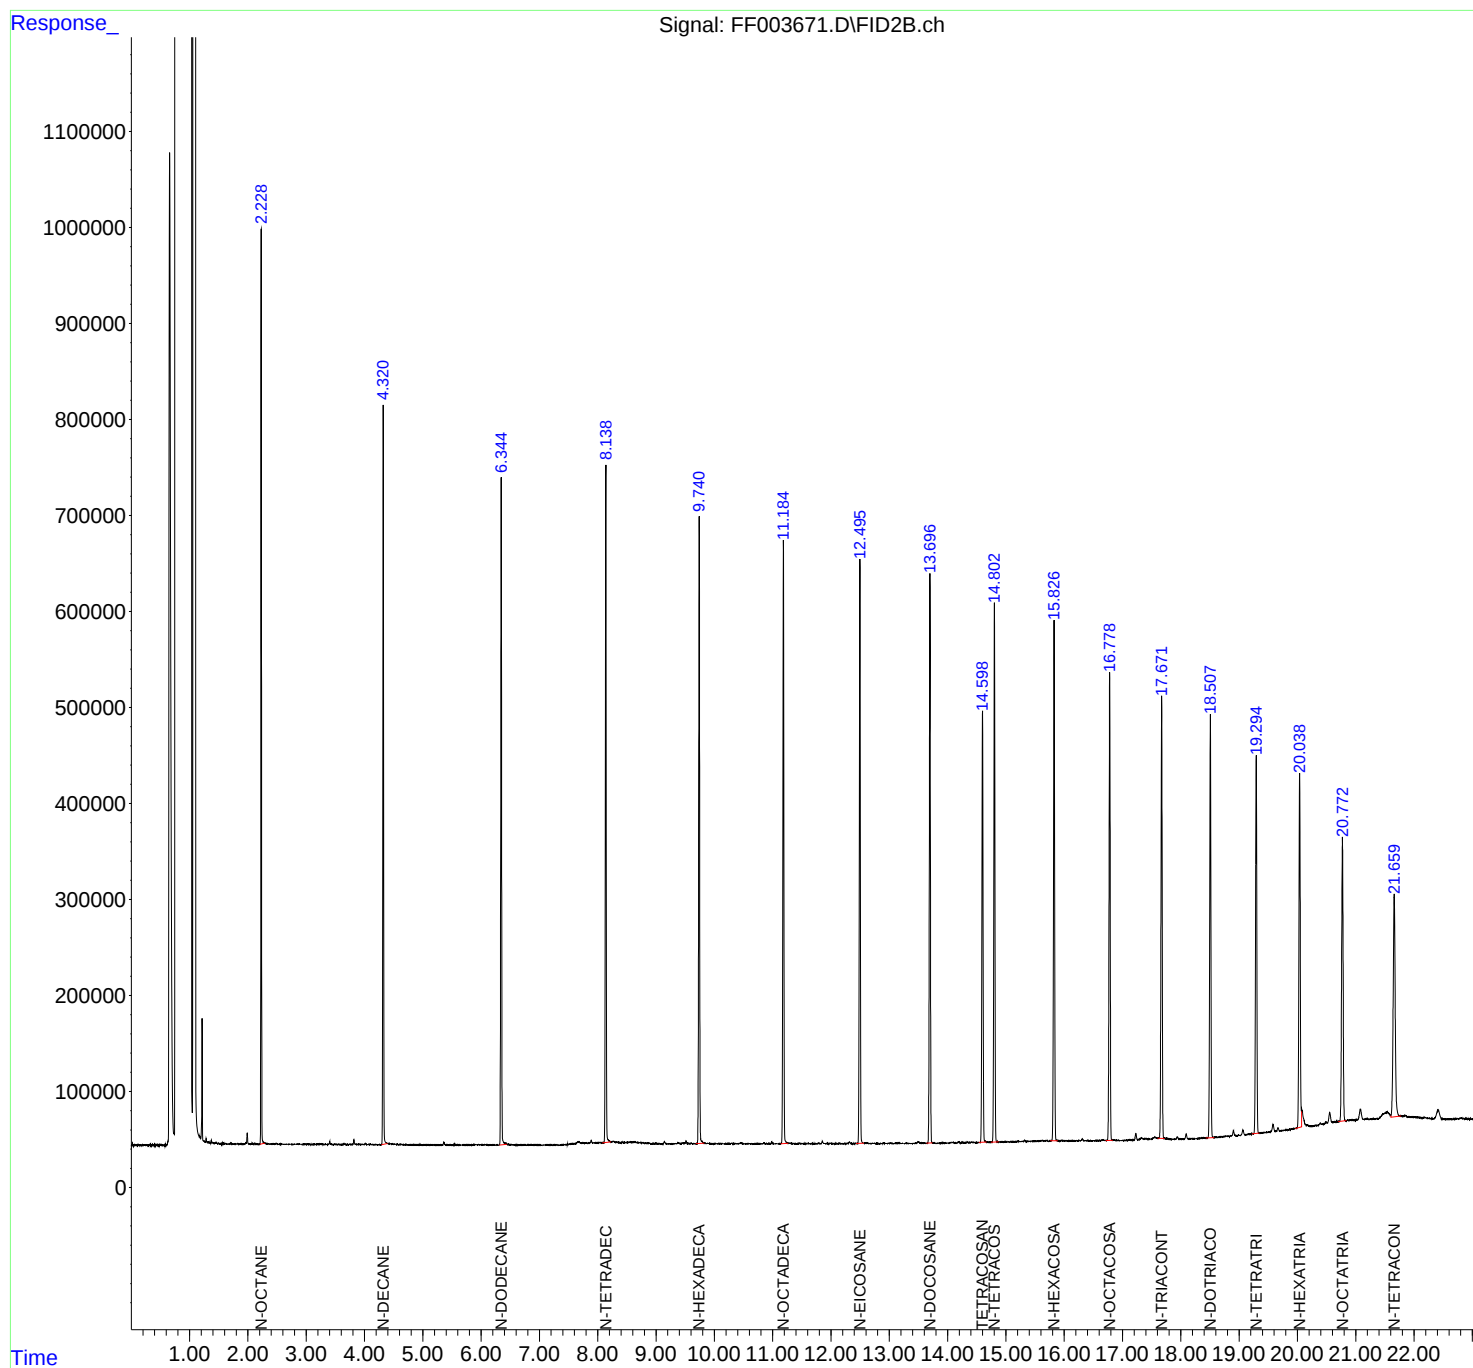


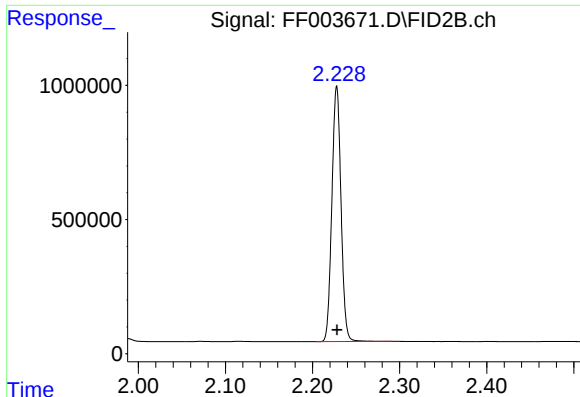

#1 N-OCTANE


R.T.: 2.228 min
Delta R.T.: 0.000 min
Response: 6930006
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

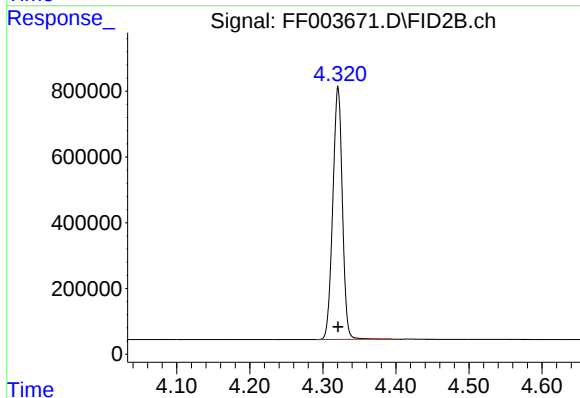


#2 N-DECANE

R.T.: 4.321 min
Delta R.T.: 0.000 min
Response: 7005449
Conc: 50.00 ug/ml

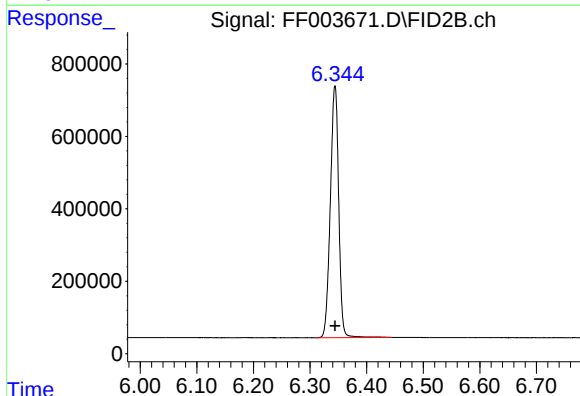


#3 N-DODECANE

R.T.: 6.344 min
Delta R.T.: 0.000 min
Response: 7139156
Conc: 50.00 ug/ml

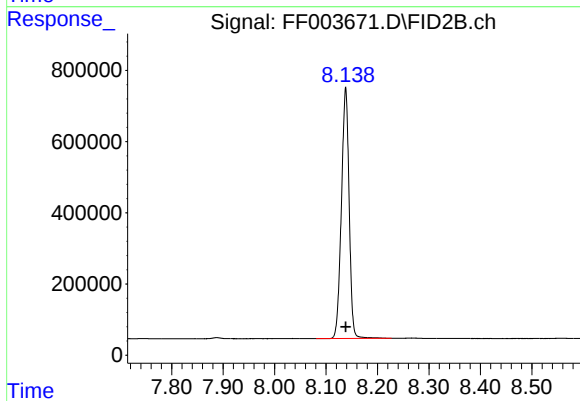

#4 N-TETRADECANE


R.T.: 8.138 min
Delta R.T.: 0.000 min
Response: 7339427
Conc: 50.00 ug/ml

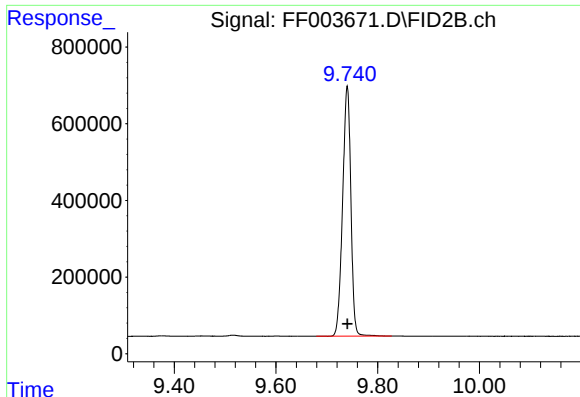

#5 N-HEXADECANE


R.T.: 9.740 min
Delta R.T.: 0.000 min
Response: 7359712
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

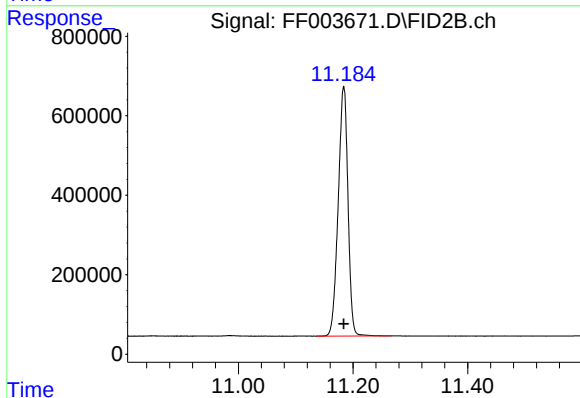


#6 N-OCTADECANE

R.T.: 11.184 min
Delta R.T.: 0.000 min
Response: 7416987
Conc: 50.00 ug/ml

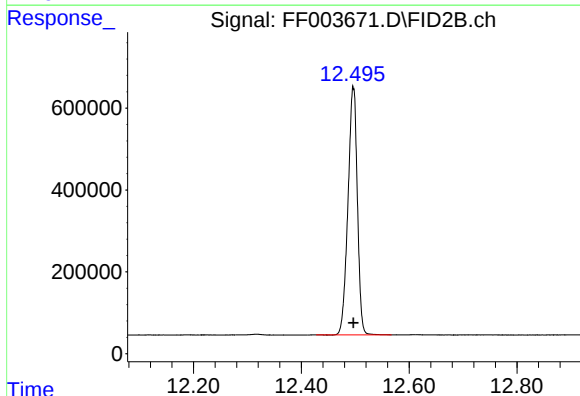


#7 N-EICOSANE

R.T.: 12.496 min
Delta R.T.: 0.000 min
Response: 7329189
Conc: 50.00 ug/ml

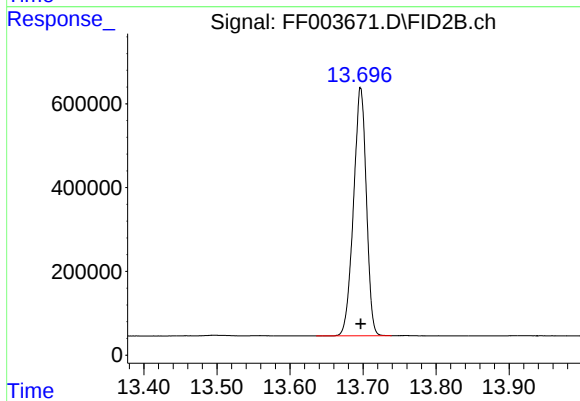

#8 N-DOCOSANE


R.T.: 13.697 min
Delta R.T.: 0.000 min
Response: 7228416
Conc: 50.00 ug/ml

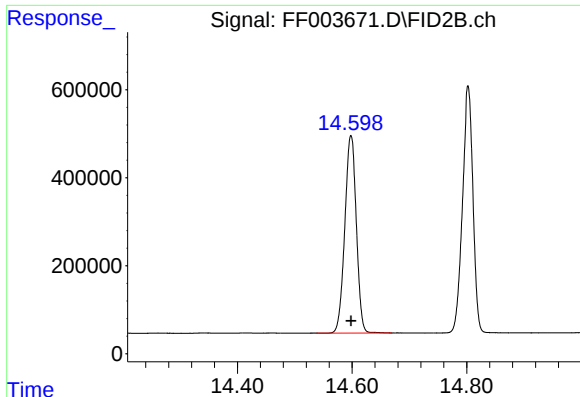

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.598 min
Delta R.T.: 0.000 min
Response: 6247747
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

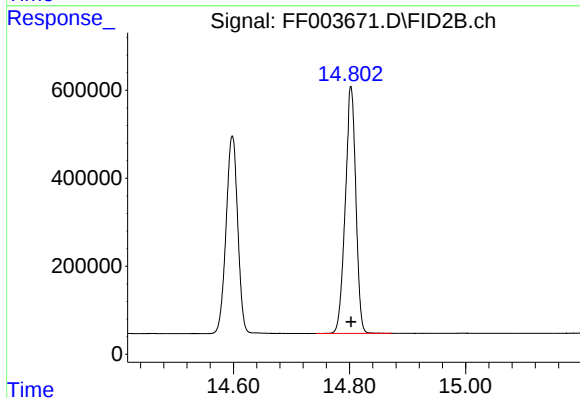


#10 N-TETRACOSANE

R.T.: 14.802 min
Delta R.T.: 0.000 min
Response: 7094457
Conc: 50.00 ug/ml

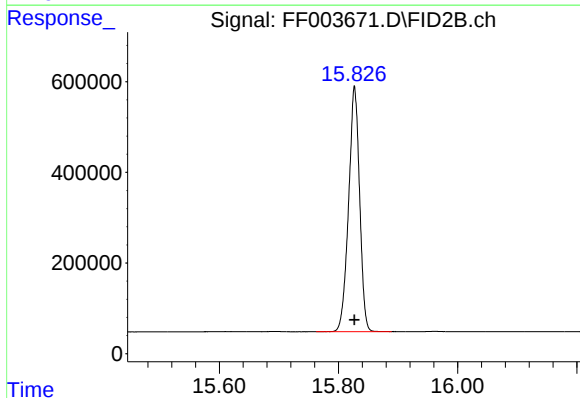


#11 N-HEXACOSANE

R.T.: 15.827 min
Delta R.T.: 0.000 min
Response: 6933857
Conc: 50.00 ug/ml

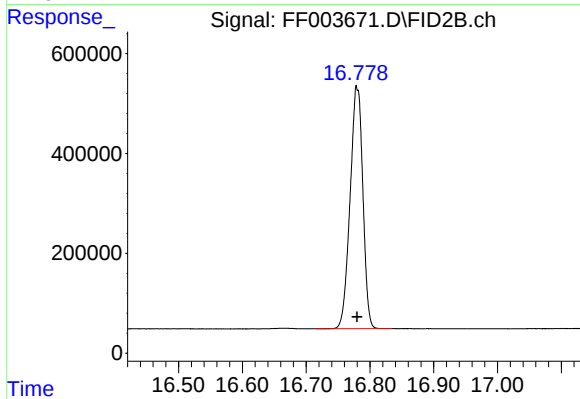

#12 N-OCTACOSANE


R.T.: 16.780 min
Delta R.T.: 0.000 min
Response: 6752974
Conc: 50.00 ug/ml

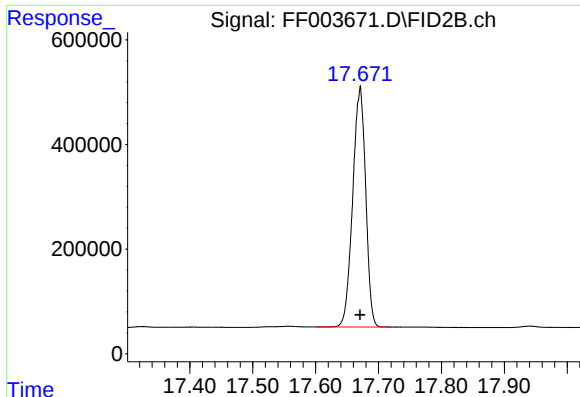

#13 N-TRIACONTANE


R.T.: 17.671 min
Delta R.T.: 0.000 min
Response: 6557888
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

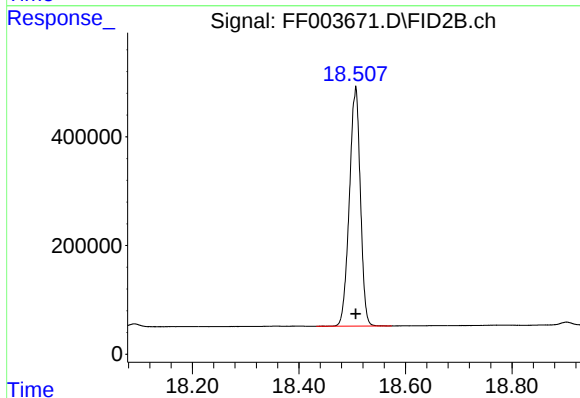


#14 N-DOTRIACONTANE

R.T.: 18.507 min
Delta R.T.: 0.000 min
Response: 6289687
Conc: 50.00 ug/ml

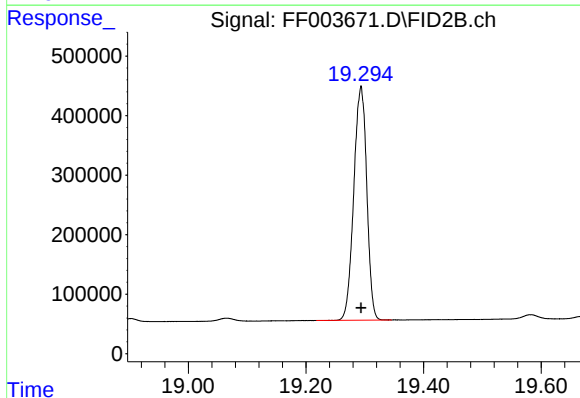


#15 N-TETRATRIACONTANE

R.T.: 19.294 min
Delta R.T.: 0.000 min
Response: 6013989
Conc: 50.00 ug/ml

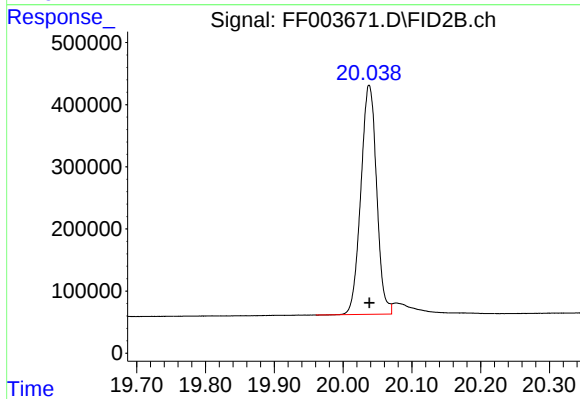

#16 N-HEXATRIACONTANE


R.T.: 20.038 min
Delta R.T.: 0.000 min
Response: 5868202
Conc: 50.00 ug/ml

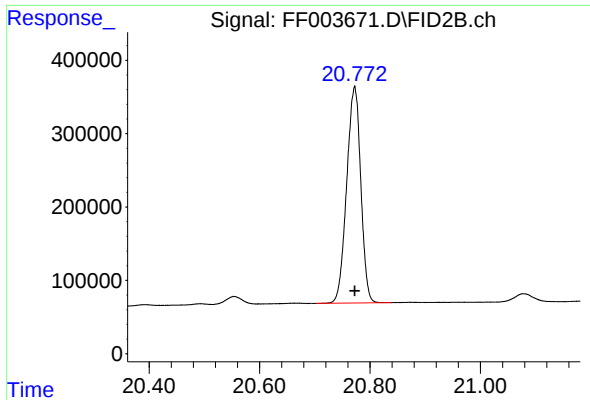

#17 N-OCTATRIACONTANE

R.T.: 20.772 min
Delta R.T.: 0.000 min
Response: 5226401
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :
50 TRPH STD

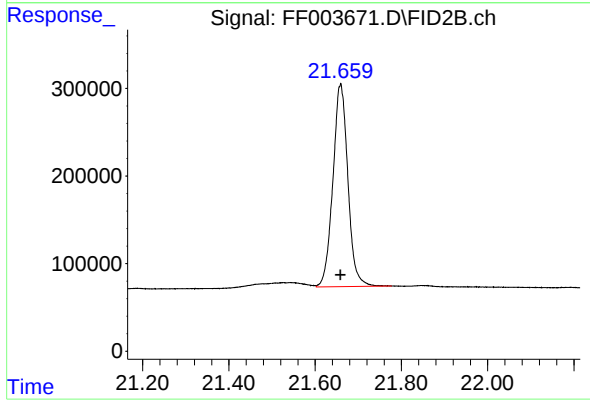

#18 N-TETRACONTANE

R.T.: 21.659 min
Delta R.T.: 0.000 min
Response: 5584387
Conc: 50.00 ug/ml