

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID\_F\Data\FF030119\  
Data File : FF003684.D  
Signal(s) : FID2B.ch  
Acq On : 01 Mar 2019 21:56  
Operator : AJ\SJ  
Sample : K1648-04  
Misc :  
ALS Vial : 60 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
SIMW-02-20190226-A

Integration File: autoint1.e  
Quant Time: Mar 04 10:20:18 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.595 | 2191031  | 15.737 ug/ml |
| Target Compounds              |        |          |              |
| 16) N-HEXATRIACONTANE         | 20.074 | 256509   | 1.966 ug/ml  |
| 18) N-TETRACONTANE            | 21.683 | 199339   | 1.602 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID\_F\Data\FF030119\  
Data File : FF003684.D  
Signal(s) : FID2B.ch  
Acq On : 01 Mar 2019 21:56  
Operator : AJ\SJ  
Sample : K1648-04  
Misc :  
ALS Vial : 60 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
SIMW-02-20190226-A

Integration File: autoint1.e  
Quant Time: Mar 04 10:20:18 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

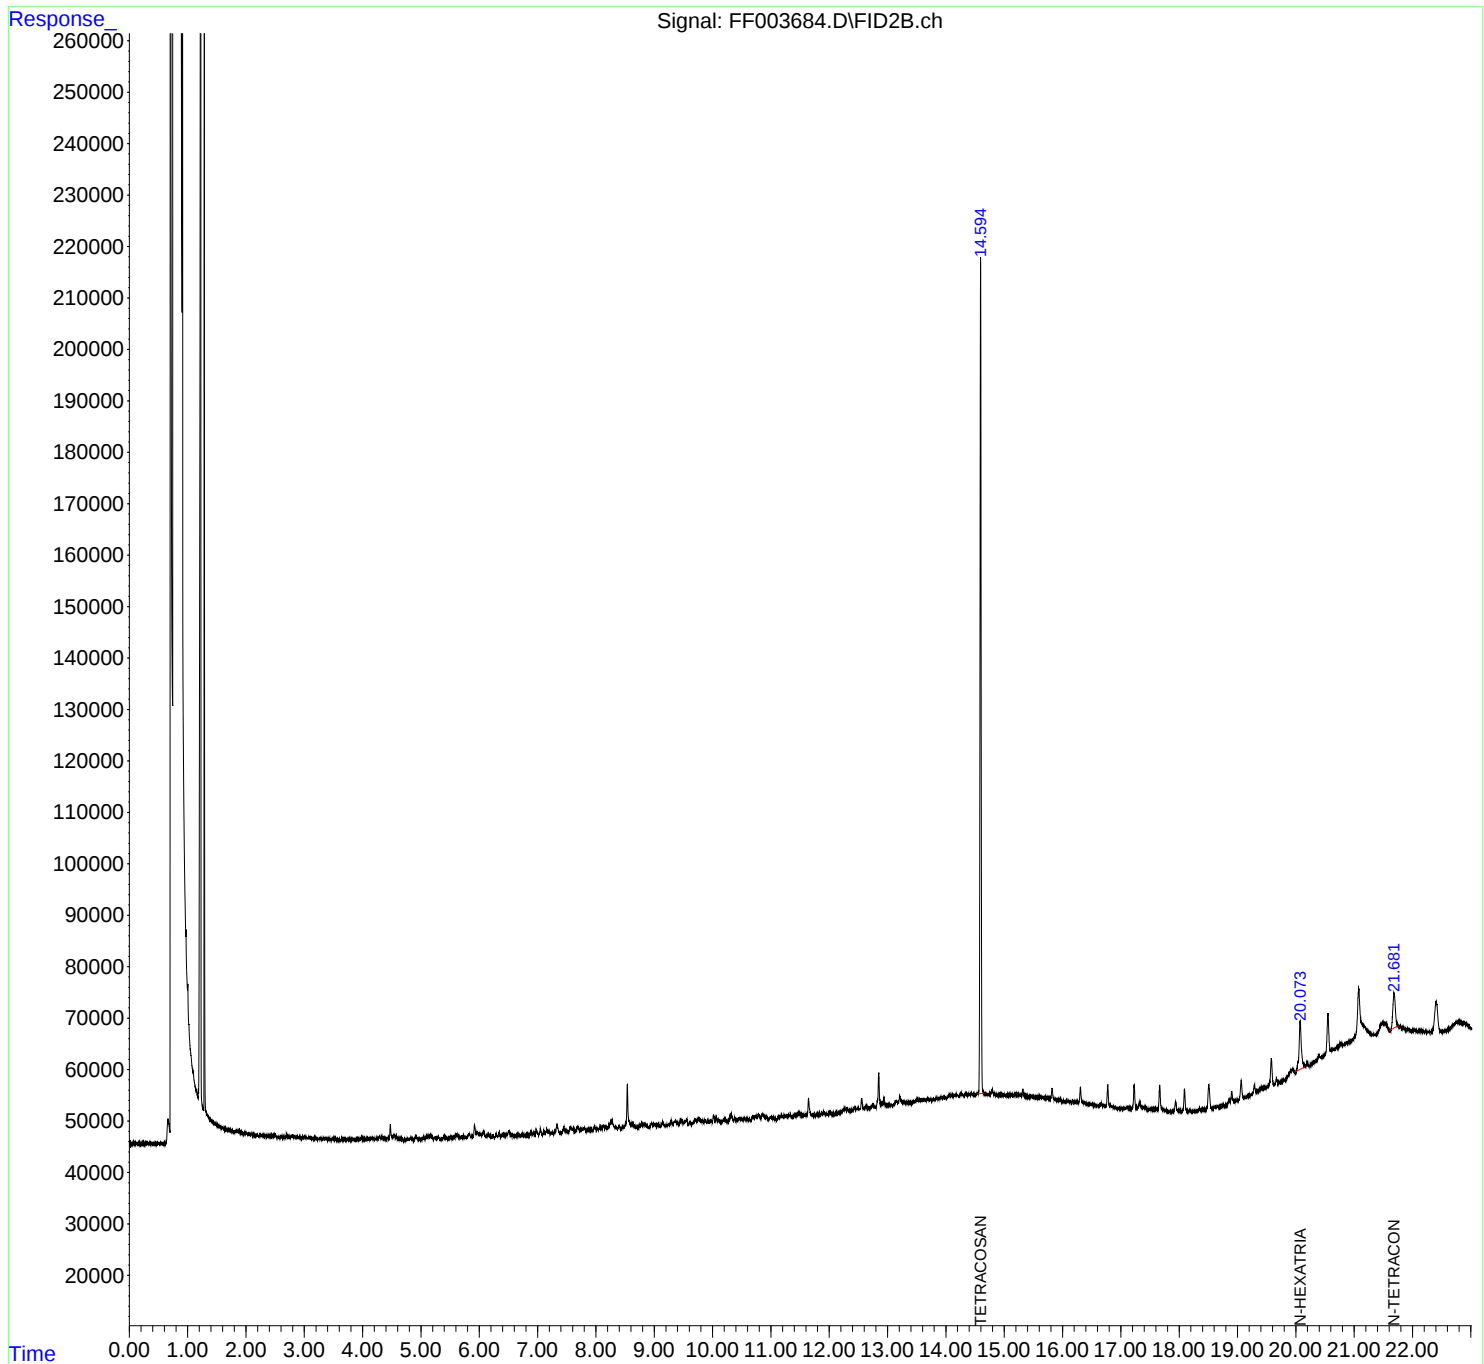


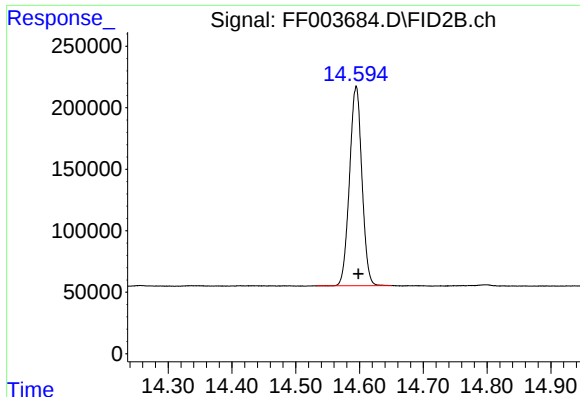

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.595 min  
Delta R.T.: -0.003 min  
Response: 2191031  
Conc: 15.74 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
SIMW-02-20190226-A

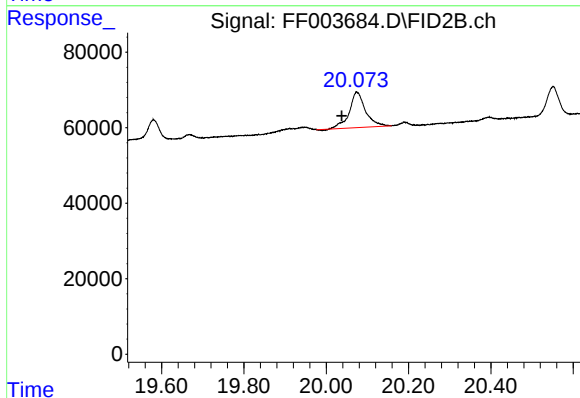

#16 N-HEXATRIACONTANE

R.T.: 20.074 min  
Delta R.T.: 0.036 min  
Response: 256509  
Conc: 1.97 ug/ml

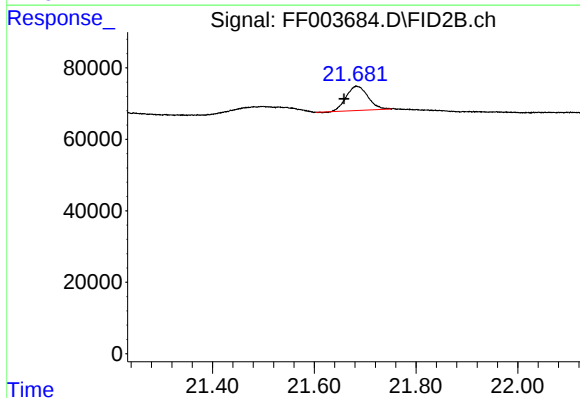

#18 N-TETRACONTANE

R.T.: 21.683 min  
Delta R.T.: 0.025 min  
Response: 199339  
Conc: 1.60 ug/ml