

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF030119\
 Data File : FF003685.D
 Signal(s) : FID2B.ch
 Acq On : 01 Mar 2019 22:26
 Operator : AJ\SJ
 Sample : K1648-05
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SIMW-04-20190226

Integration File: autoint1.e
 Quant Time: Mar 04 10:20:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.595	2633517	18.915 ug/ml
Target Compounds			
2) N-DECANE	4.264f	298834	1.943 ug/ml
3) N-DODECANE	6.332	750789	4.811 ug/ml
4) N-TETRADECANE	8.161	973598	6.072 ug/ml
5) N-HEXADECANE	9.762	970426	5.958 ug/ml
6) N-OCTADECANE	11.177	701062	4.255 ug/ml
7) N-EICOSANE	12.557f	261562	1.599 ug/ml
13) N-TRIACONTANE	17.664	116294	0.791 ug/ml
14) N-DOTRIACONTANE	18.512	274200	1.928 ug/ml
16) N-HEXATRIACONTANE	20.074	755295	5.789 ug/ml
18) N-TETRACONTANE	21.684	953986	7.668 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF030119\
Data File : FF003685.D
Signal(s) : FID2B.ch
Acq On : 01 Mar 2019 22:26
Operator : AJ\SJ
Sample : K1648-05
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SIMW-04-20190226

Integration File: autoint1.e
Quant Time: Mar 04 10:20:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

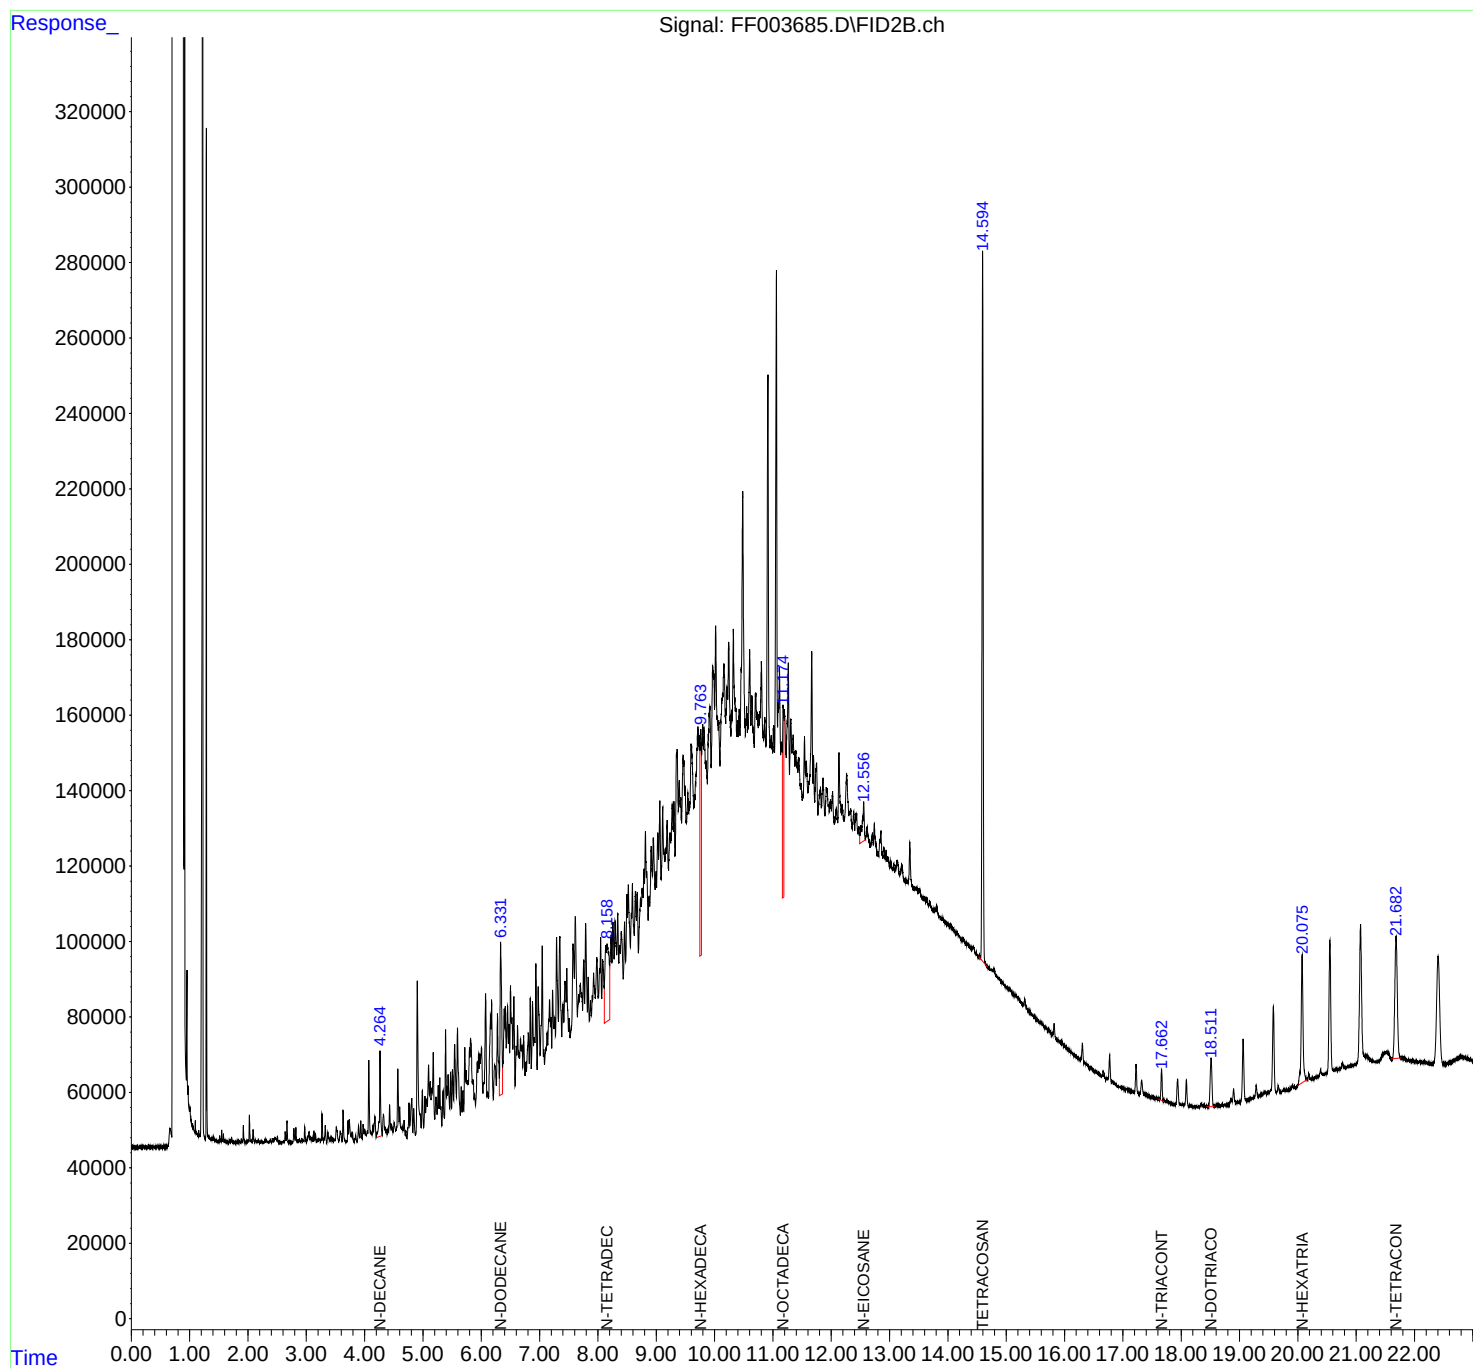


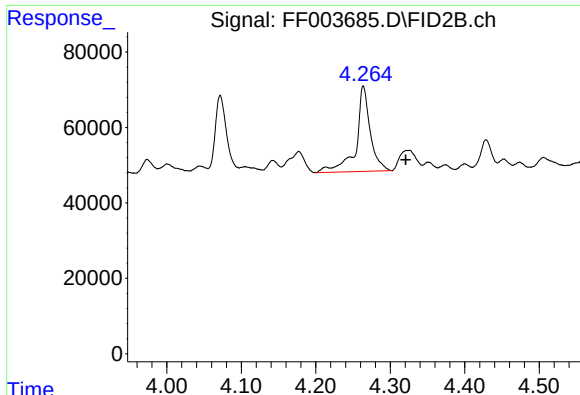

#2 N-DECANE


R.T.: 4.264 min
Delta R.T.: -0.057 min
Response: 298834
Conc: 1.94 ug/ml

Instrument :
FID_F
ClientSampleId :
SIMW-04-20190226

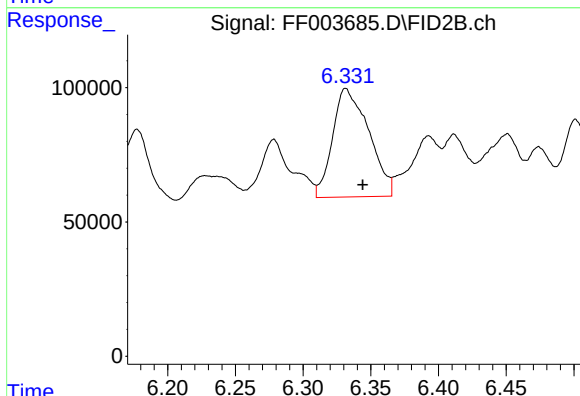


#3 N-DODECANE

R.T.: 6.332 min
Delta R.T.: -0.012 min
Response: 750789
Conc: 4.81 ug/ml

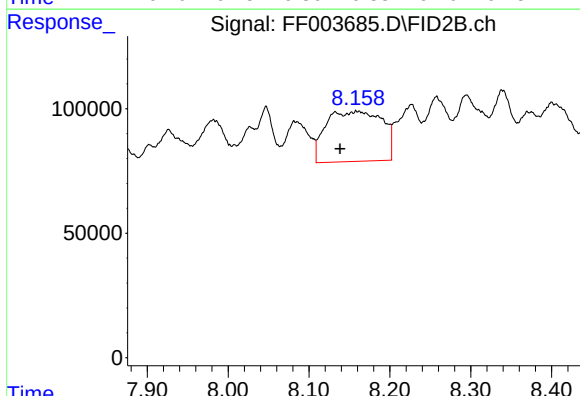


#4 N-TETRADECANE

R.T.: 8.161 min
Delta R.T.: 0.022 min
Response: 973598
Conc: 6.07 ug/ml

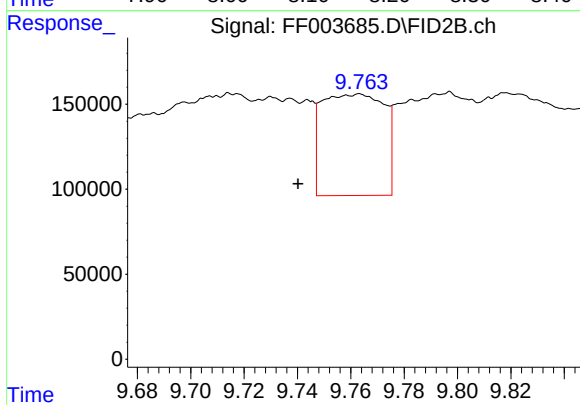

#5 N-HEXADECANE


R.T.: 9.762 min
Delta R.T.: 0.022 min
Response: 970426
Conc: 5.96 ug/ml

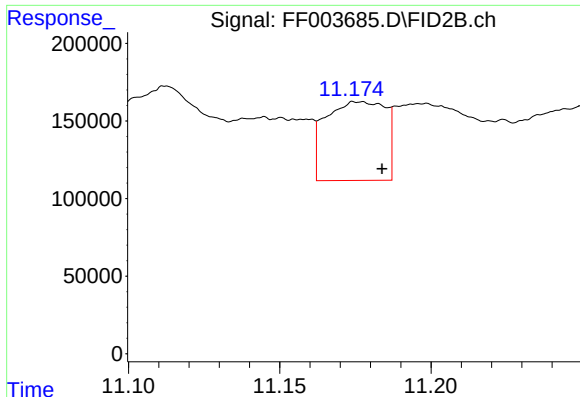

#6 N-OCTADECANE


R.T.: 11.177 min
Delta R.T.: -0.007 min
Response: 701062
Conc: 4.26 ug/ml

Instrument :
FID_F
ClientSampleId :
SIMW-04-20190226

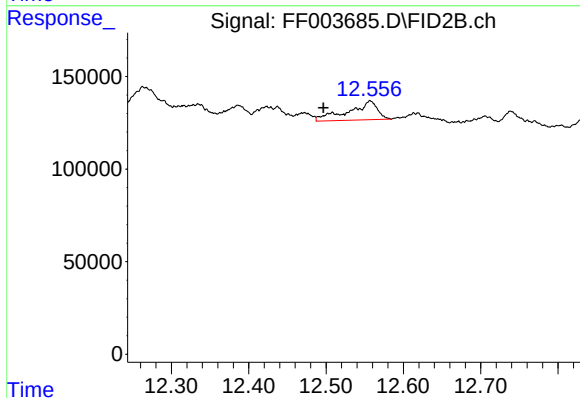


#7 N-EICOSANE

R.T.: 12.557 min
Delta R.T.: 0.061 min
Response: 261562
Conc: 1.60 ug/ml

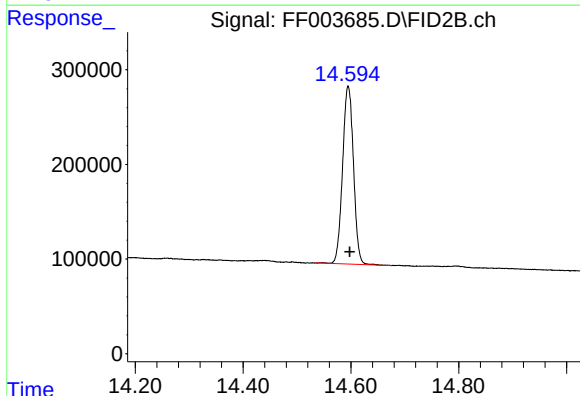


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.595 min
Delta R.T.: -0.003 min
Response: 2633517
Conc: 18.92 ug/ml

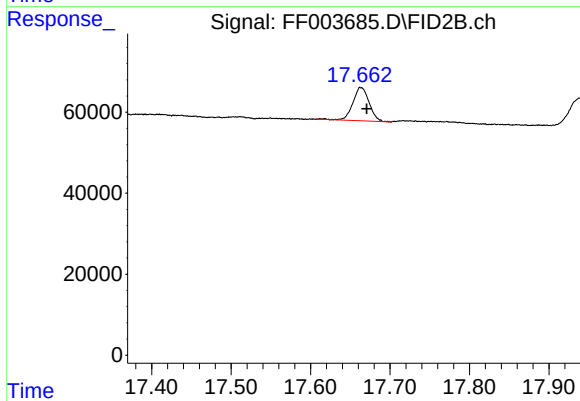

#13 N-TRIACONTANE


R.T.: 17.664 min
Delta R.T.: -0.007 min
Response: 116294
Conc: 0.79 ug/ml

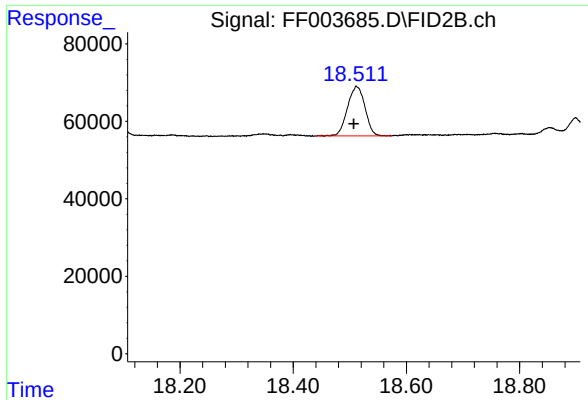

#14 N-DOTRIACONTANE


R.T.: 18.512 min
Delta R.T.: 0.006 min
Response: 274200
Conc: 1.93 ug/ml

Instrument :
FID_F
ClientSampleId :
SIMW-04-20190226

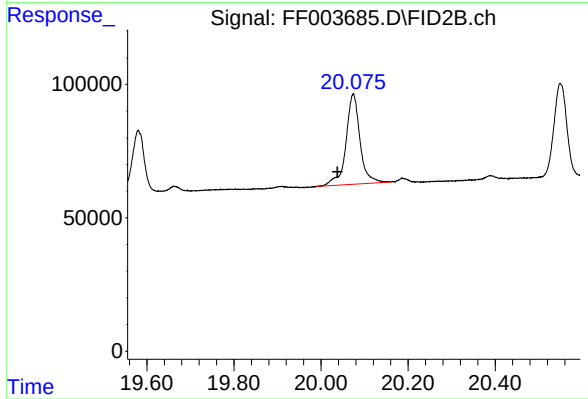

#16 N-HEXATRIACONTANE

R.T.: 20.074 min
Delta R.T.: 0.036 min
Response: 755295
Conc: 5.79 ug/ml

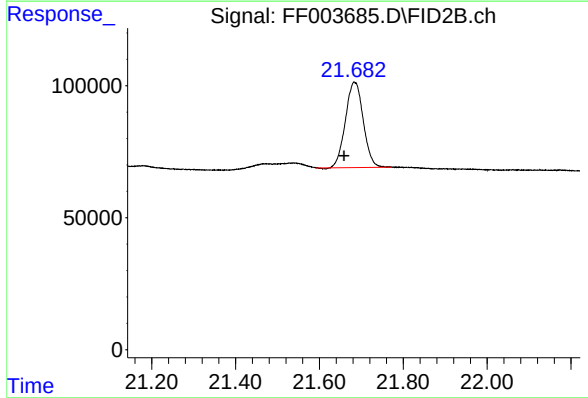

#18 N-TETRACONTANE

R.T.: 21.684 min
Delta R.T.: 0.025 min
Response: 953986
Conc: 7.67 ug/ml