

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF030119\
Data File : FF003687.D
Signal(s) : FID2B.ch
Acq On : 01 Mar 2019 23:26
Operator : AJ\SJ
Sample : K1648-07
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EB-20190226

Integration File: autoint1.e
Quant Time: Mar 04 10:20:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.596	2853648	20.496 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.510	141062	0.992 ug/ml
16) N-HEXATRIACONTANE	20.080	1920854	14.721 ug/ml
18) N-TETRACONTANE	21.686	411674	3.309 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF030119\
Data File : FF003687.D
Signal(s) : FID2B.ch
Acq On : 01 Mar 2019 23:26
Operator : AJ\SJ
Sample : K1648-07
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EB-20190226

Integration File: autoint1.e
Quant Time: Mar 04 10:20:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

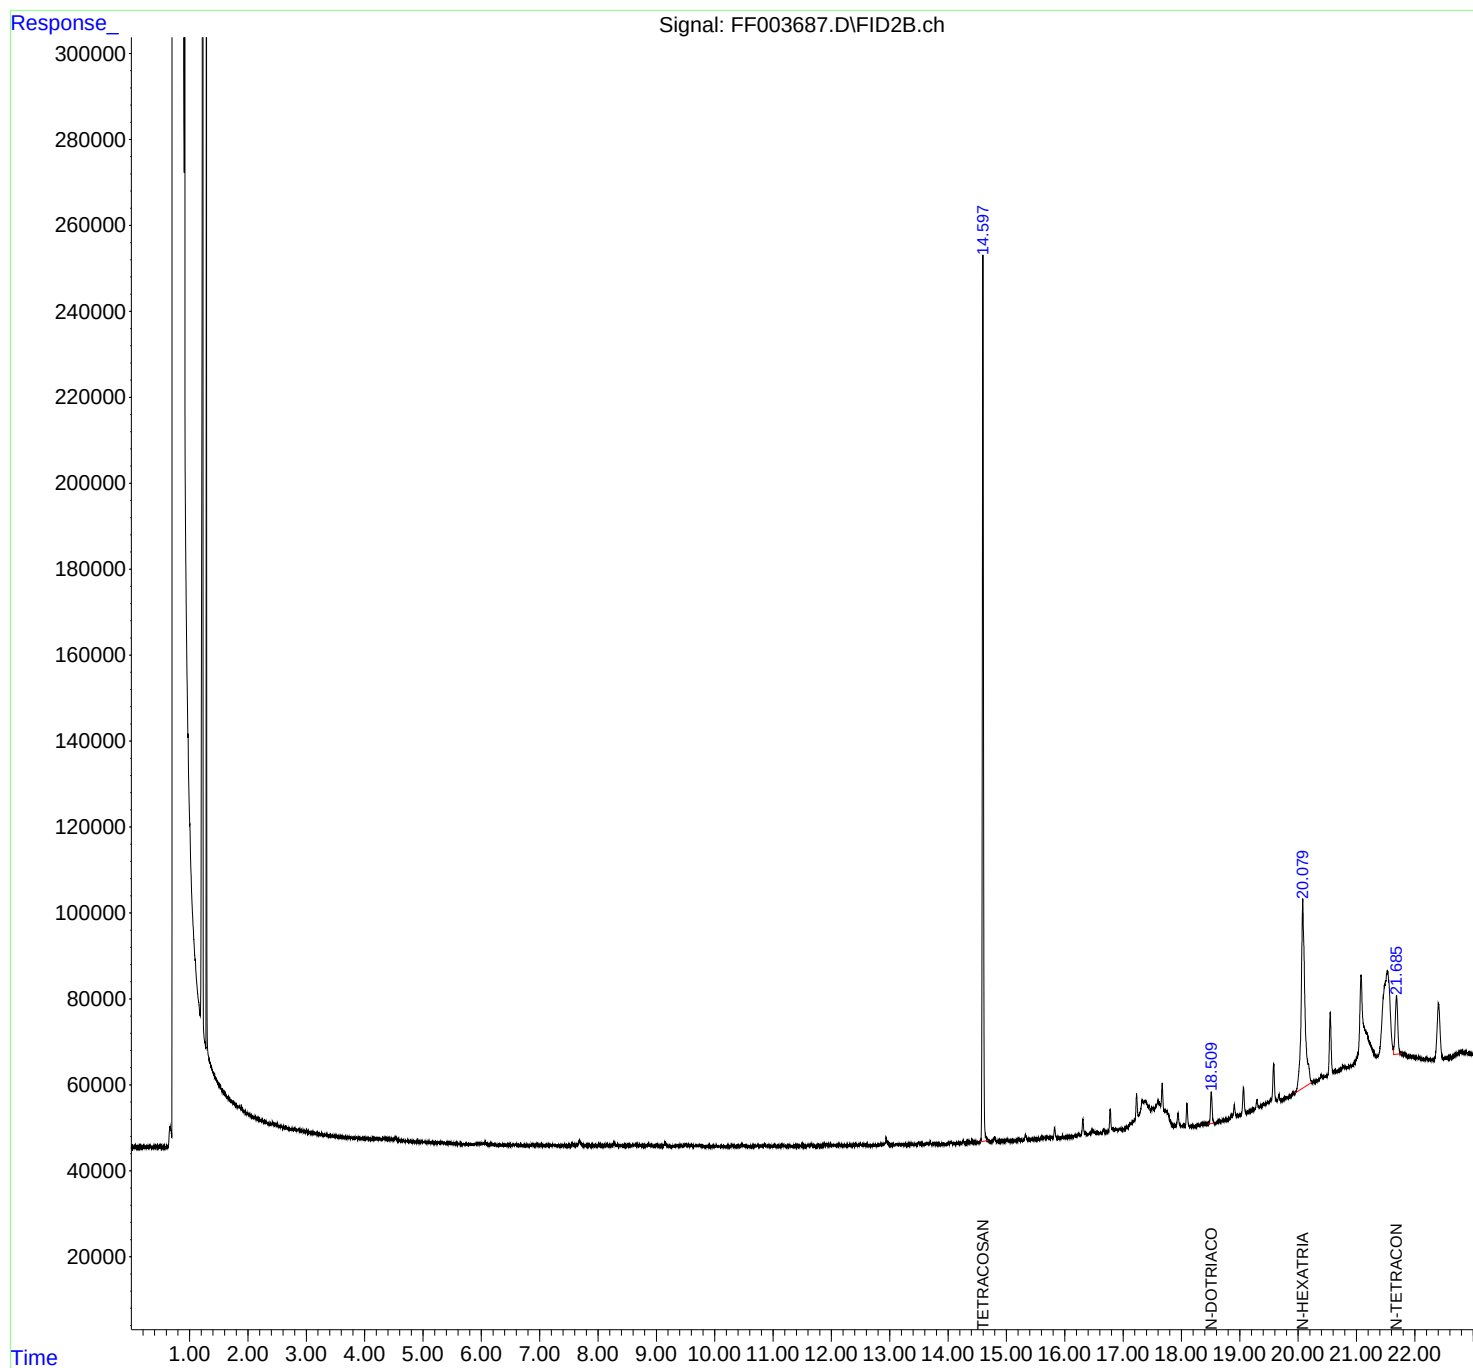


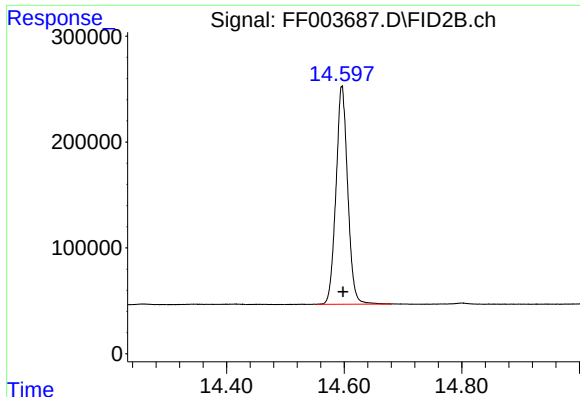

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.596 min
Delta R.T.: -0.002 min
Response: 2853648
Conc: 20.50 ug/ml

Instrument :
FID_F
ClientSampleId :
EB-20190226

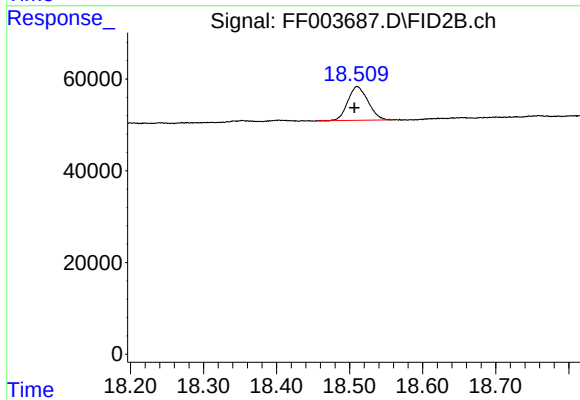


#14 N-DOTRIACONTANE

R.T.: 18.510 min
Delta R.T.: 0.004 min
Response: 141062
Conc: 0.99 ug/ml

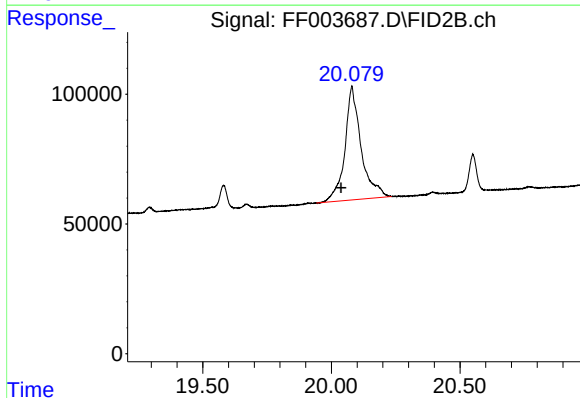

#16 N-HEXATRIACONTANE

R.T.: 20.080 min
Delta R.T.: 0.042 min
Response: 1920854
Conc: 14.72 ug/ml

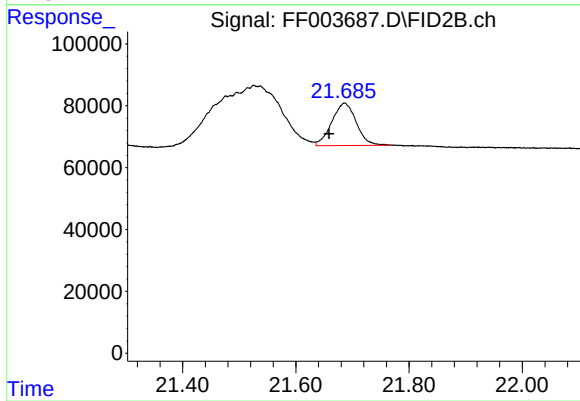

#18 N-TETRACONTANE

R.T.: 21.686 min
Delta R.T.: 0.027 min
Response: 411674
Conc: 3.31 ug/ml