

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
 Data File : FF006470.D
 Signal(s) : FID2B.ch
 Acq On : 02 Mar 2020 12:45
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 03 00:51:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.368	3687784	26.983 ug/ml
10) N-TETRACOSANE	14.771	443596	3.175 ug/ml
12) N-OCTACOSANE	16.757	3392448	24.582 ug/ml
13) N-TRIACONTANE	17.639	244557	1.768 ug/ml
14) N-DOTRIACONTANE	18.469	270383	2.055 ug/ml
15) N-TETRATRIACONTANE	19.249	181675	1.618 ug/ml
16) N-HEXATRIACONTANE	19.988	216878	2.241 ug/ml
17) N-OCTATRIACONTANE	20.707	118666	1.680 ug/ml
18) N-TETRACONTANE	21.576	202649	2.871 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
Data File : FF006470.D
Signal(s) : FID2B.ch
Acq On : 02 Mar 2020 12:45
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 00:51:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

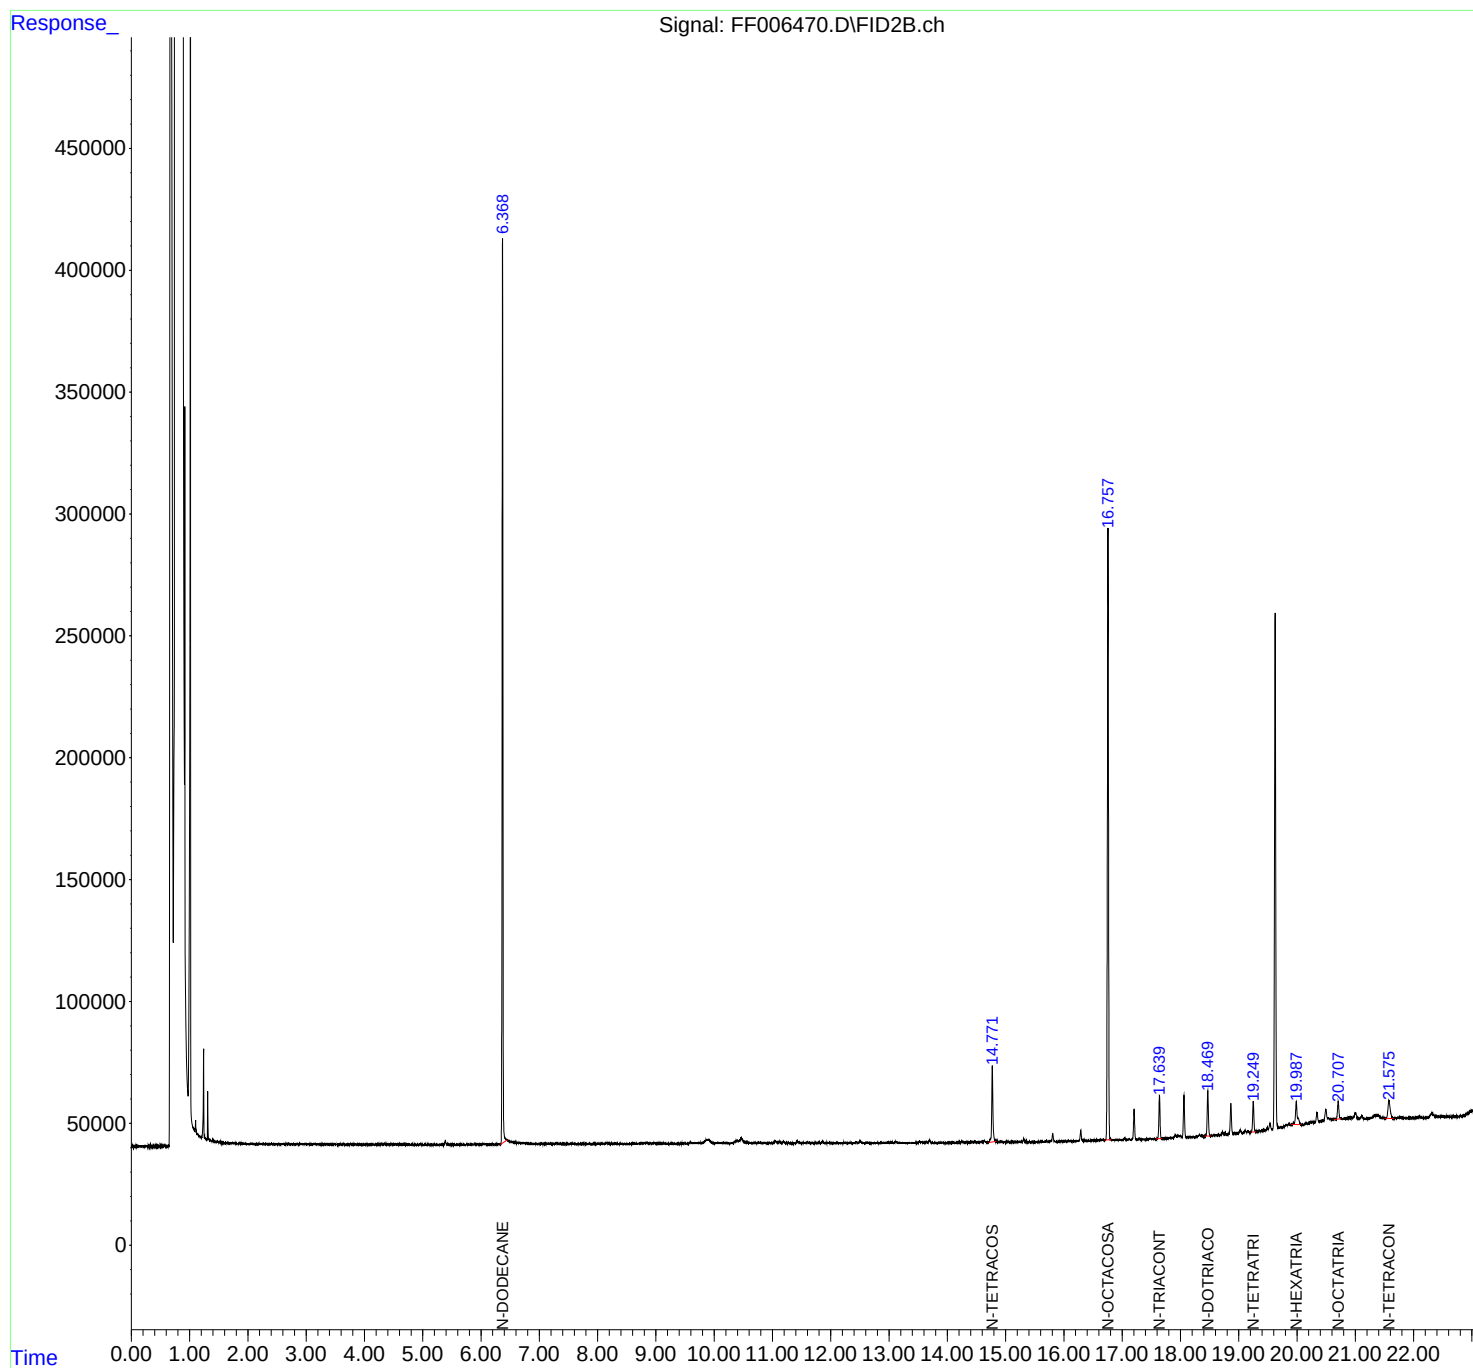


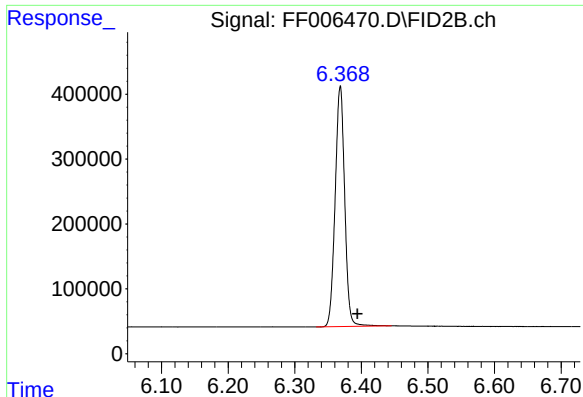

#3 N-DODECANE


R.T.: 6.368 min
Delta R.T.: -0.026 min
Response: 3687784
Conc: 26.98 ug/ml

Instrument :
FID_F
ClientSampleId :

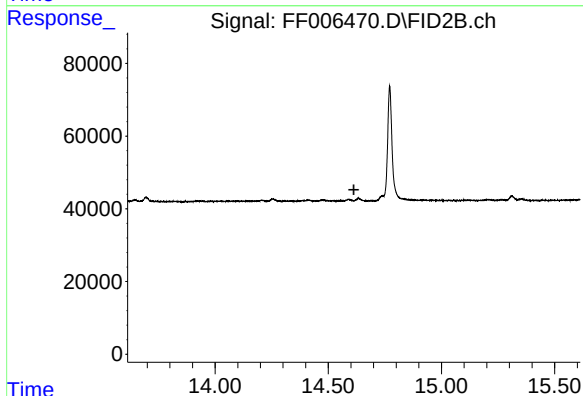


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.613 min
Response: 0
Conc: N.D.

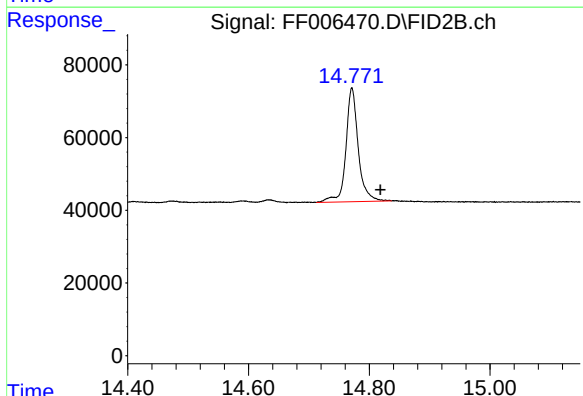


#10 N-TETRACOSANE

R.T.: 14.771 min
Delta R.T.: -0.047 min
Response: 443596
Conc: 3.17 ug/ml

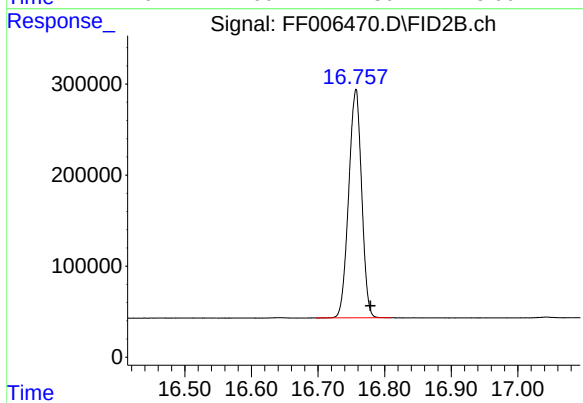

#12 N-OCTACOSANE


R.T.: 16.757 min
Delta R.T.: -0.022 min
Response: 3392448
Conc: 24.58 ug/ml

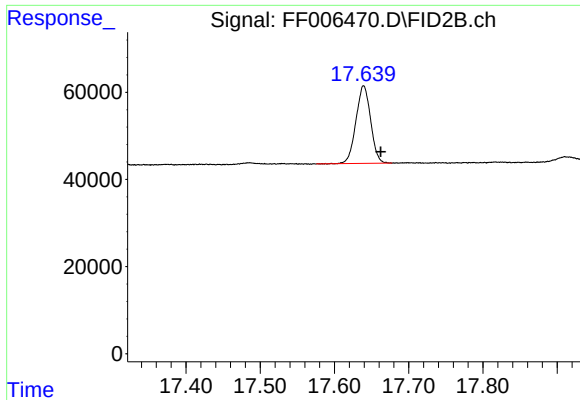

#13 N-TRIACONTANE


R.T.: 17.639 min
Delta R.T.: -0.023 min
Response: 244557
Conc: 1.77 ug/ml

Instrument :
FID_F
ClientSampleId :

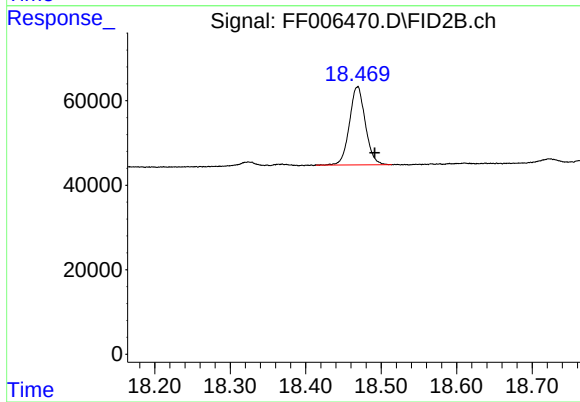


#14 N-DOTRIACONTANE

R.T.: 18.469 min
Delta R.T.: -0.023 min
Response: 270383
Conc: 2.06 ug/ml

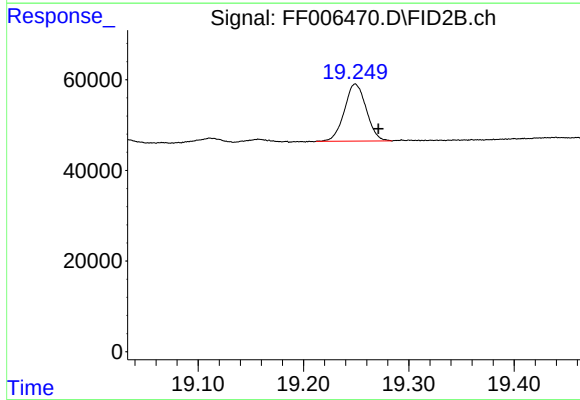


#15 N-TETRATRIACONTANE

R.T.: 19.249 min
Delta R.T.: -0.022 min
Response: 181675
Conc: 1.62 ug/ml

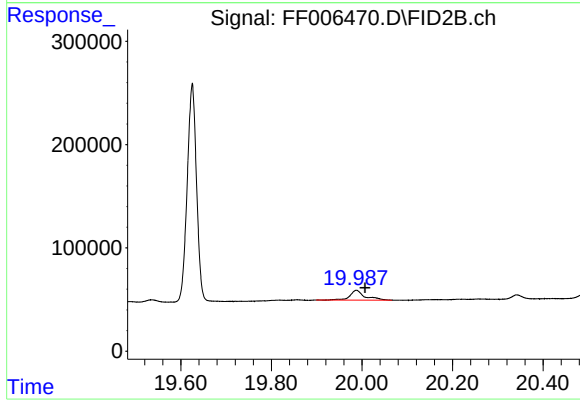

#16 N-HEXATRIACONTANE


R.T.: 19.988 min
Delta R.T.: -0.019 min
Response: 216878
Conc: 2.24 ug/ml

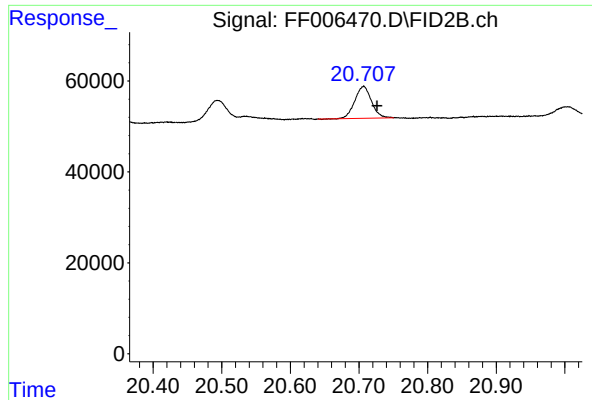

#17 N-OCTATRIACONTANE

R.T.: 20.707 min
Delta R.T.: -0.019 min
Response: 118666
Conc: 1.68 ug/ml

Instrument :
FID_F
ClientSampleId :

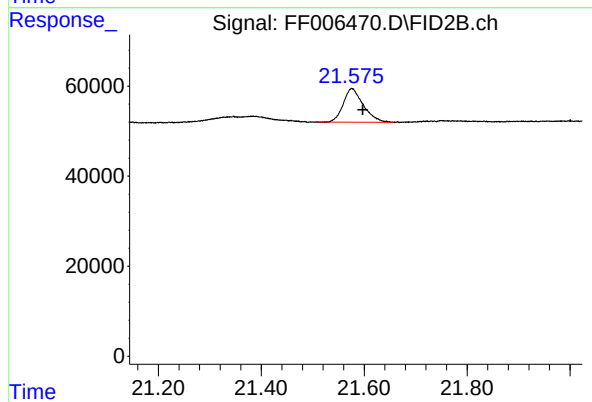

#18 N-TETRACONTANE

R.T.: 21.576 min
Delta R.T.: -0.021 min
Response: 202649
Conc: 2.87 ug/ml